

ORL-063

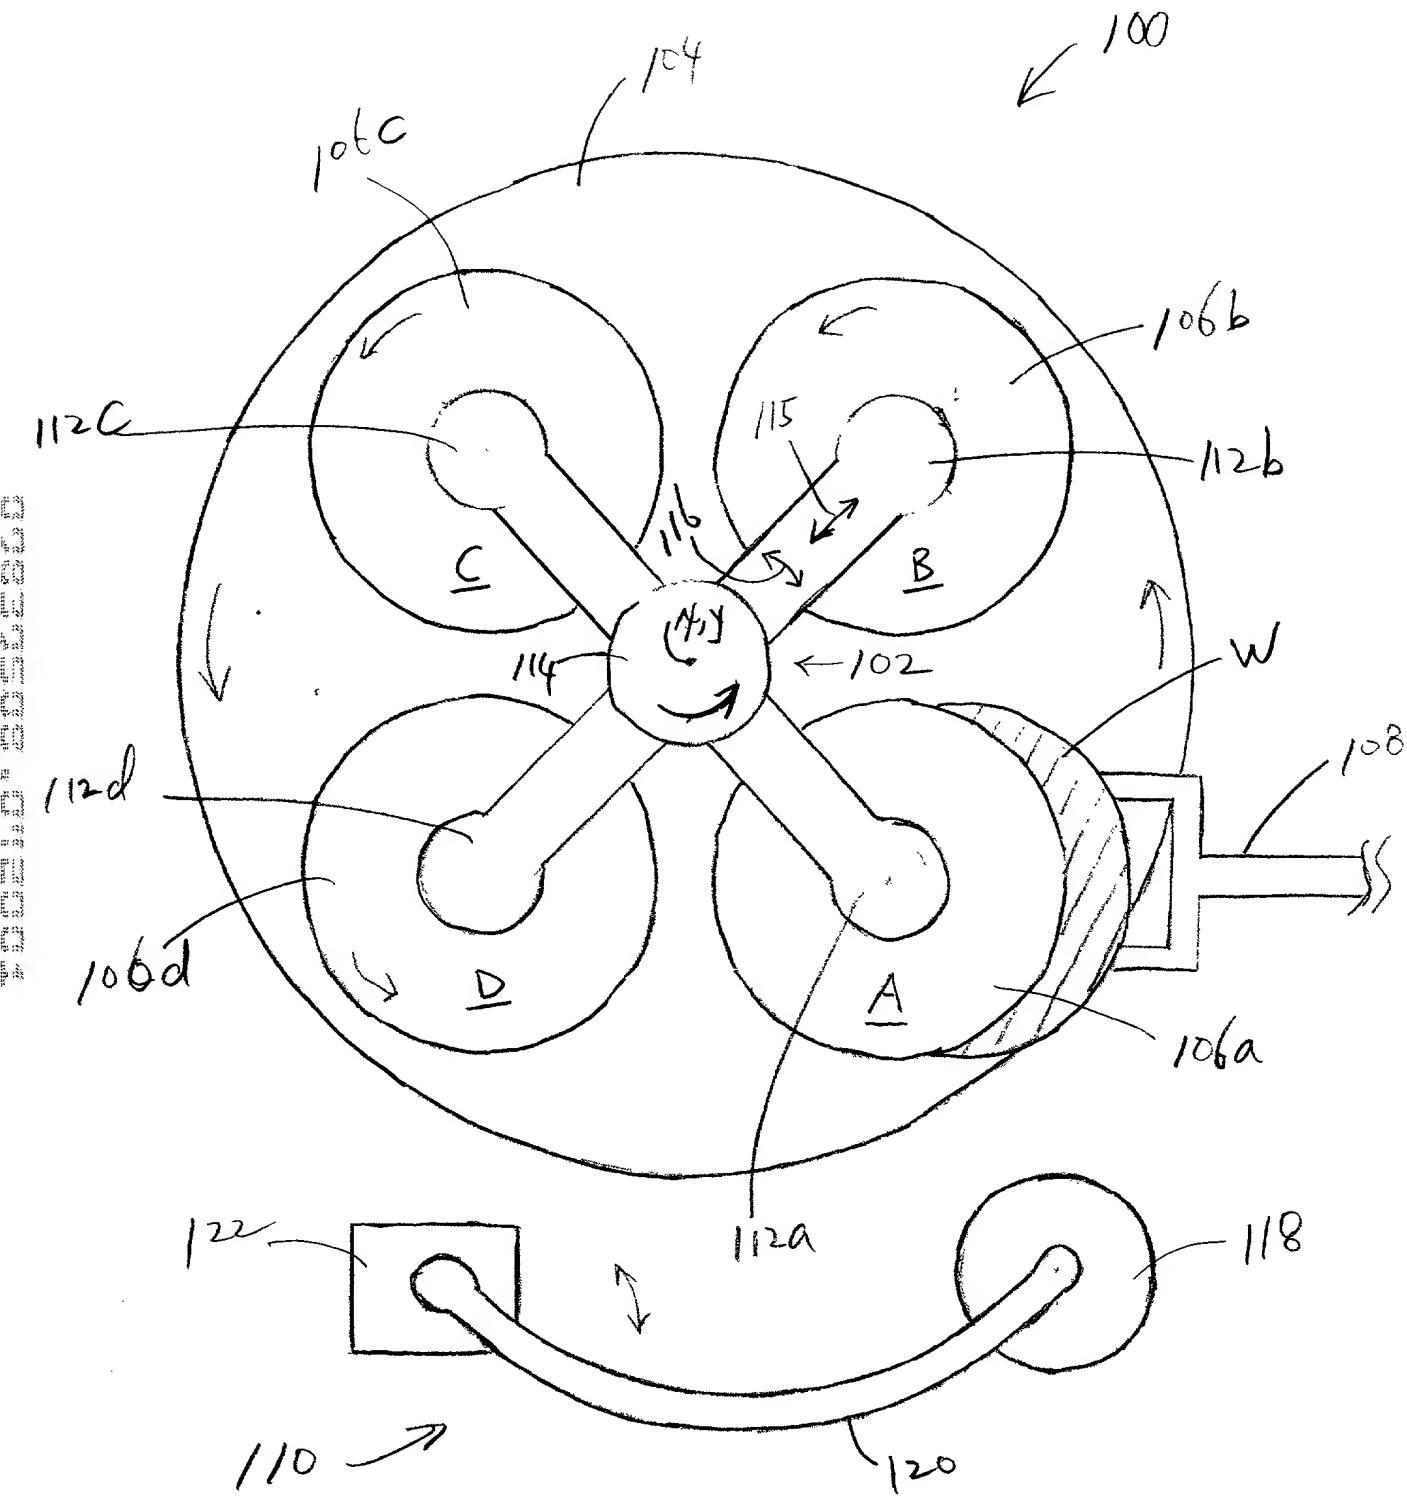


FIG. 1

ORL-003

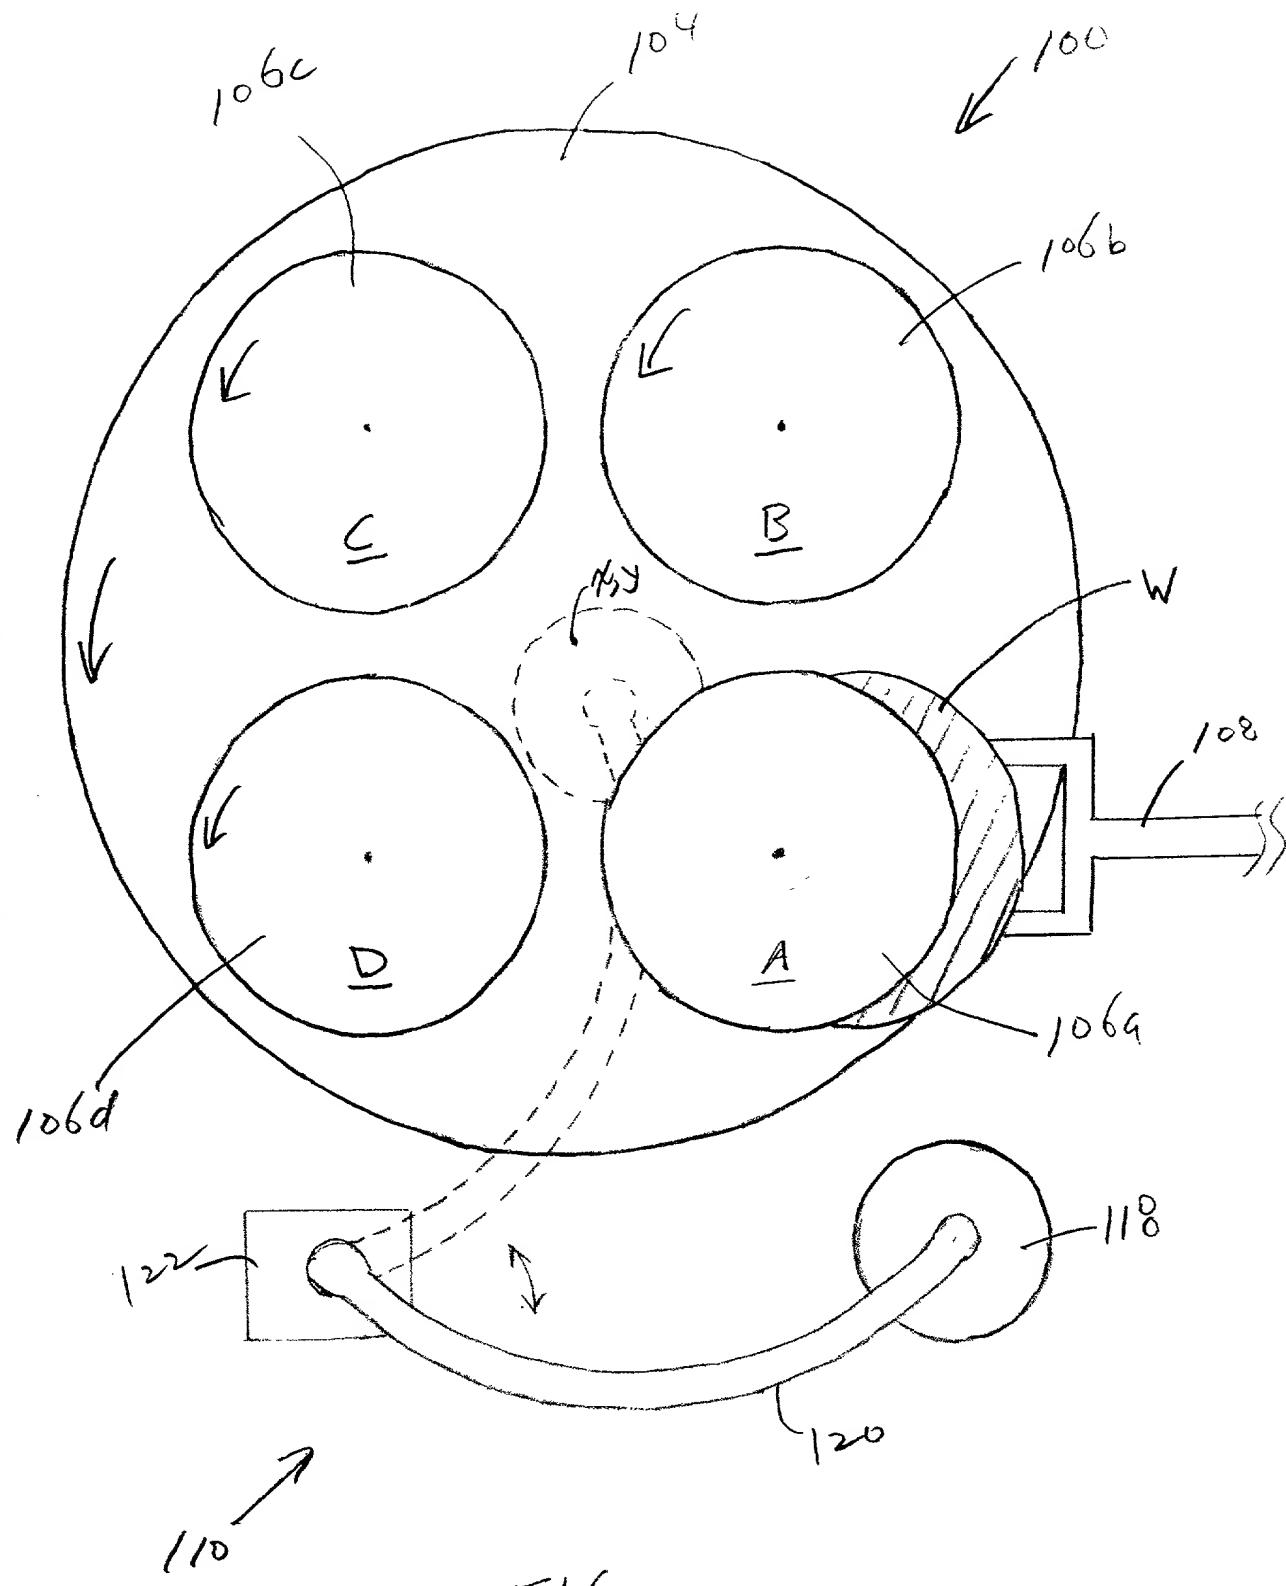


FIG. 2

6RL-003

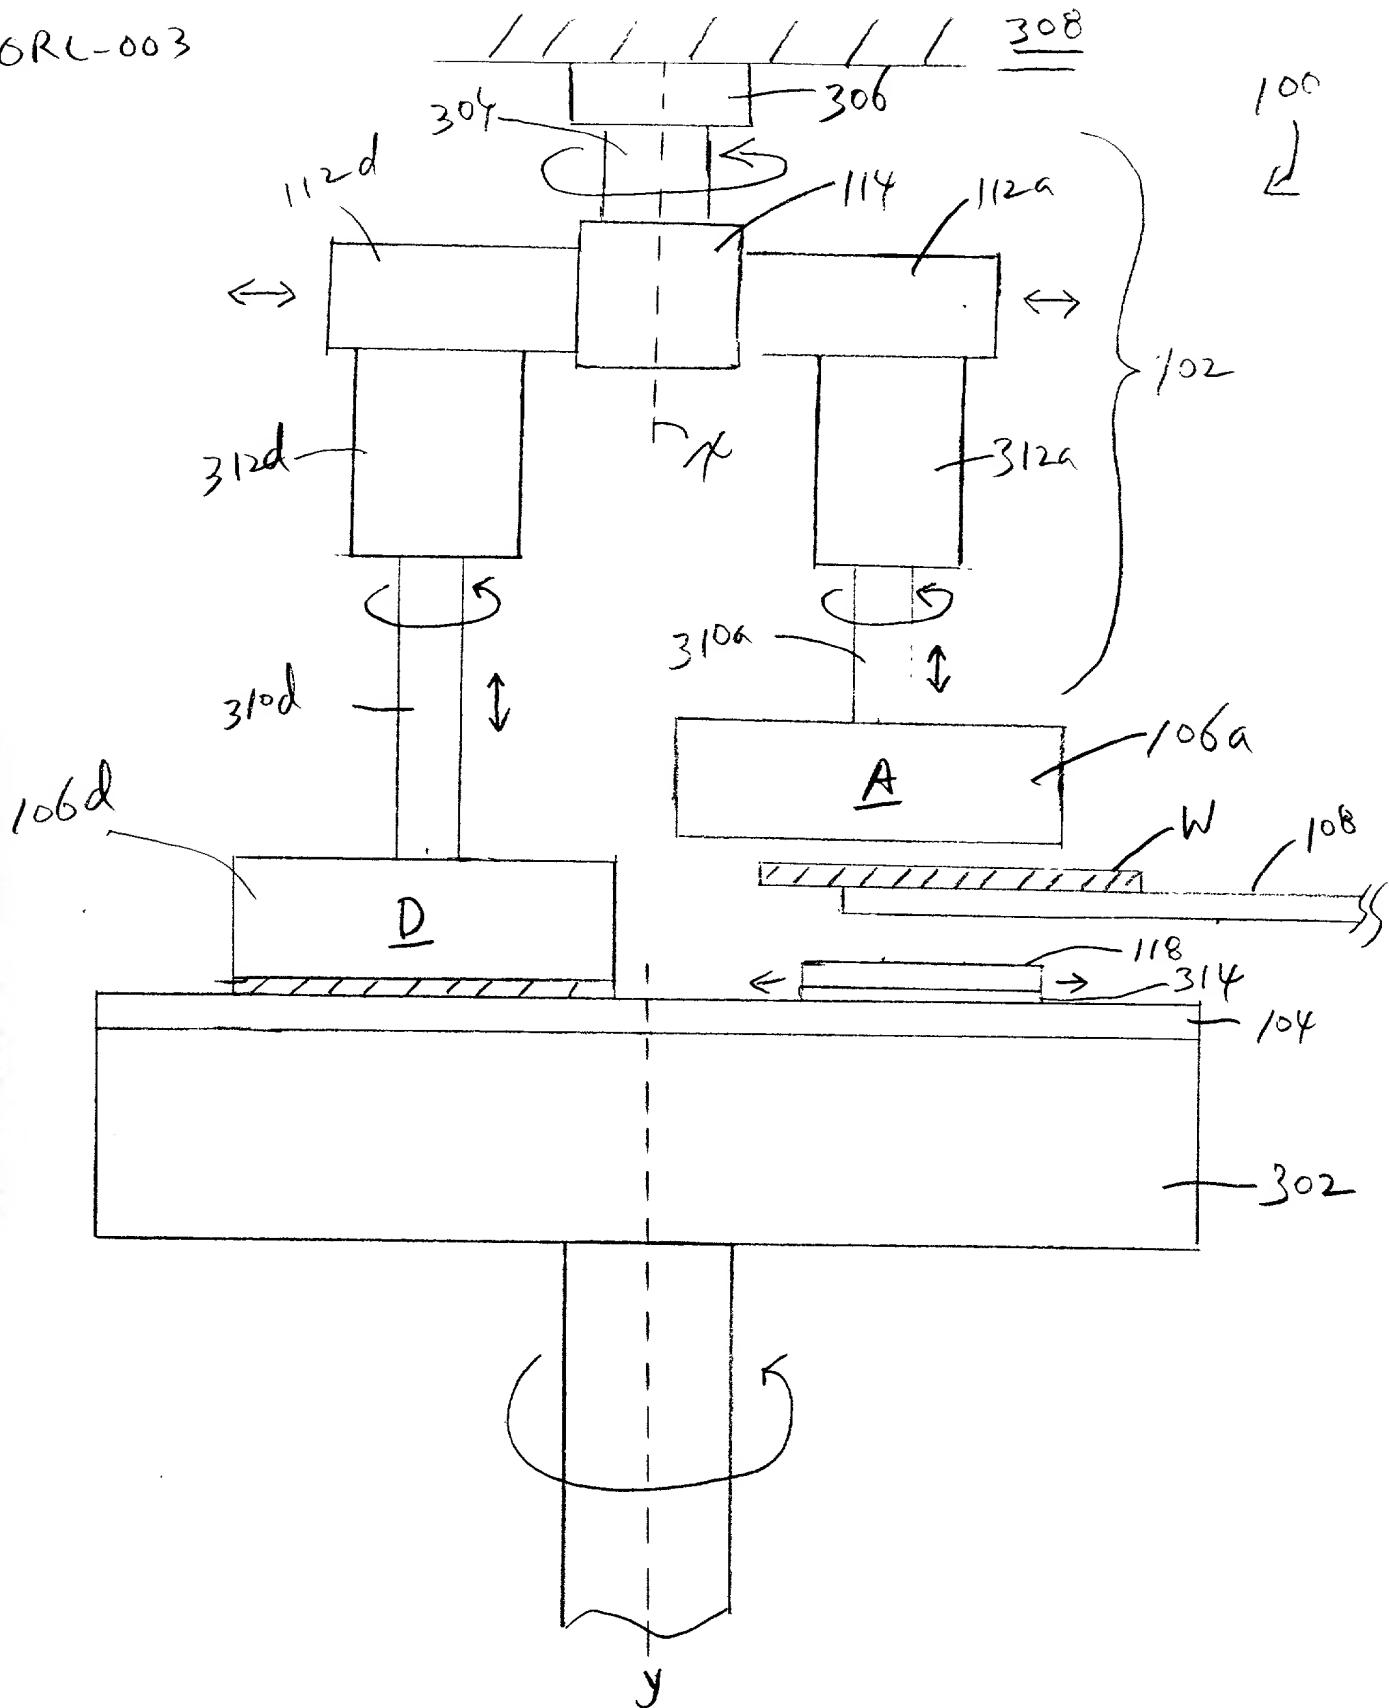


FIG. 3

ORL-003






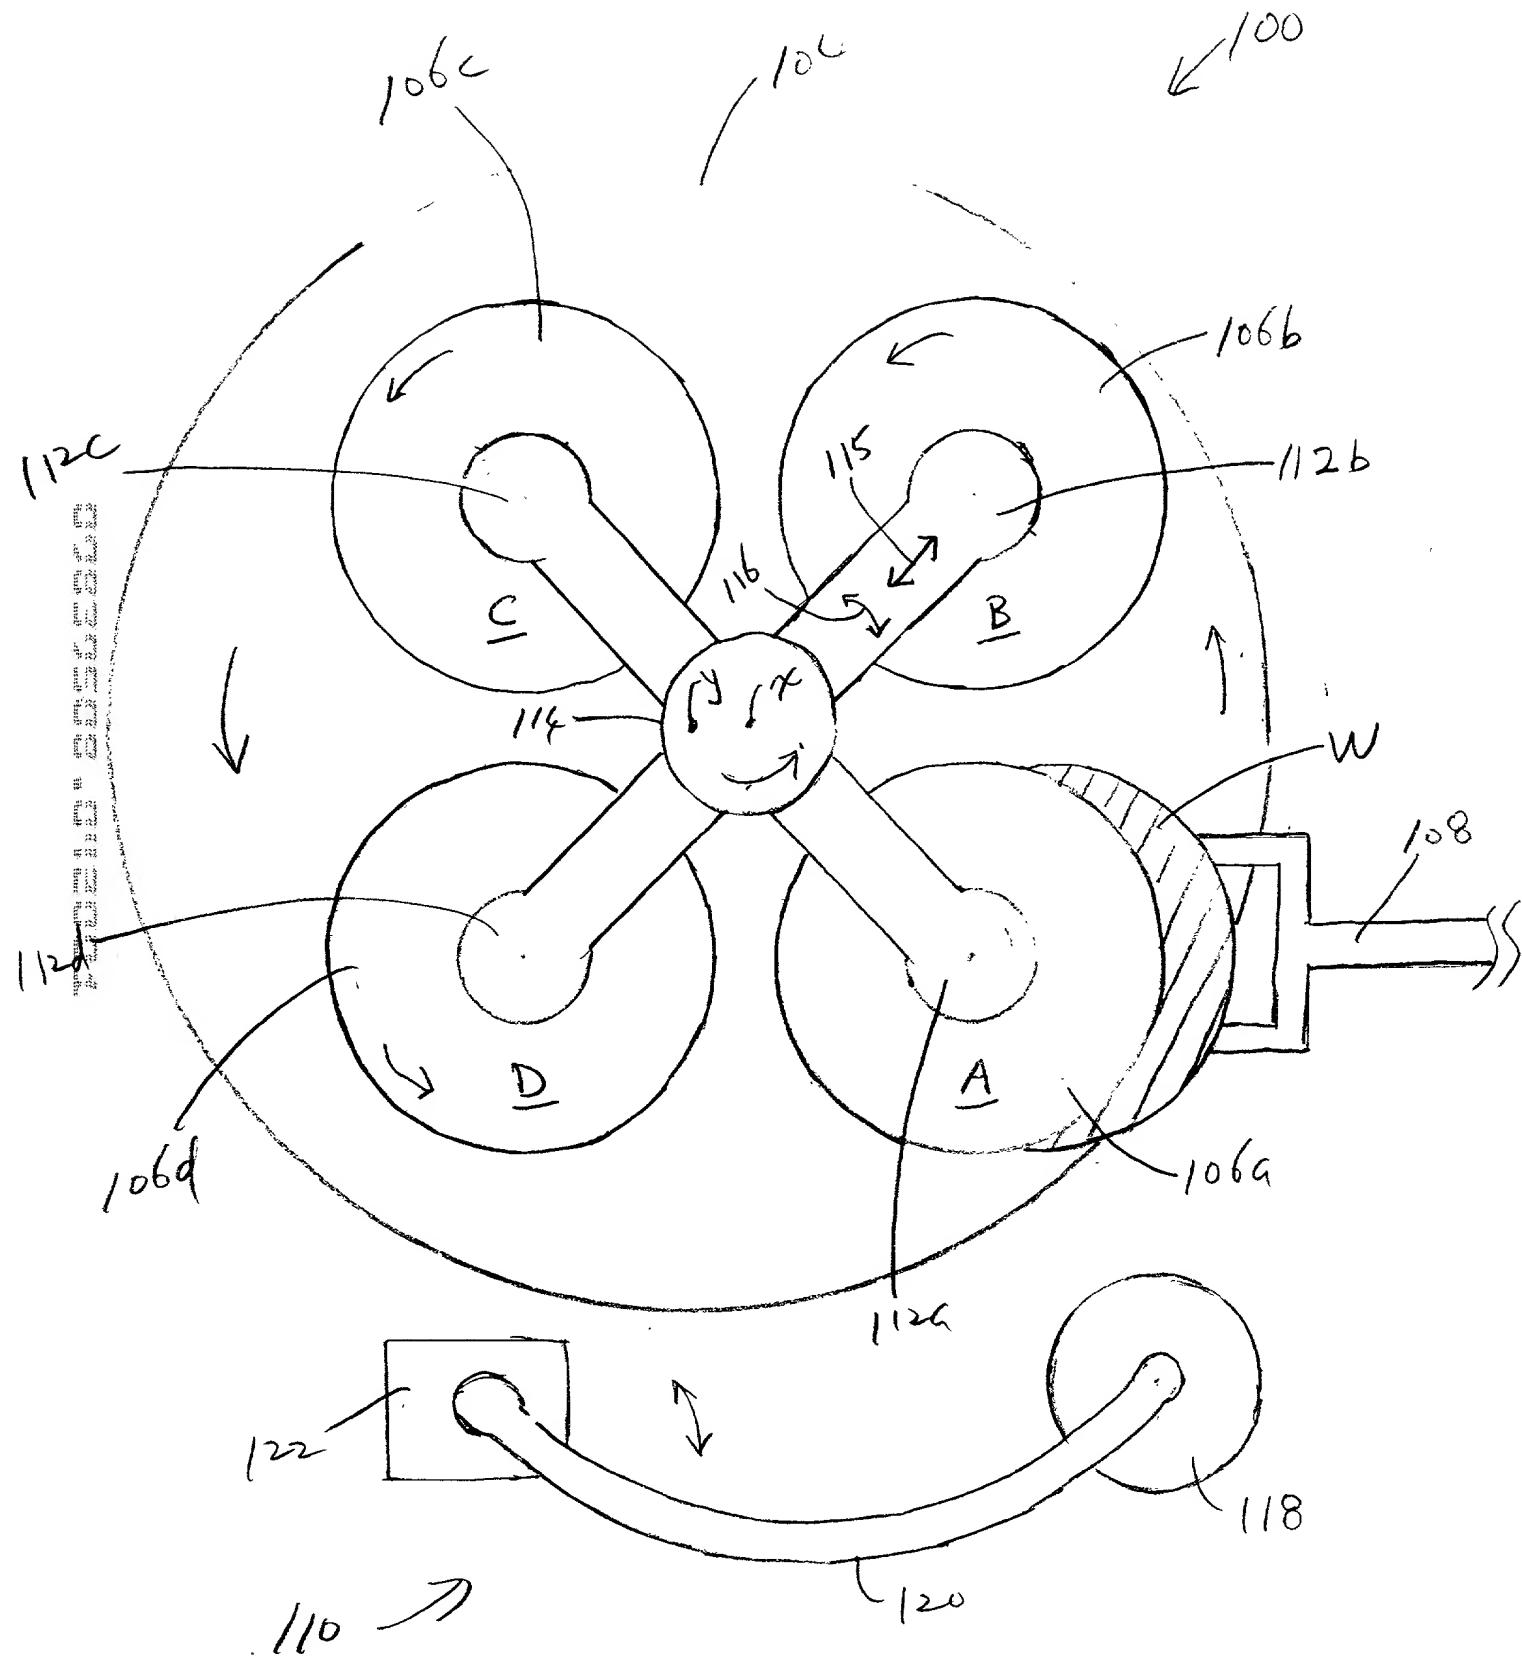


FIG.4

ORL-003

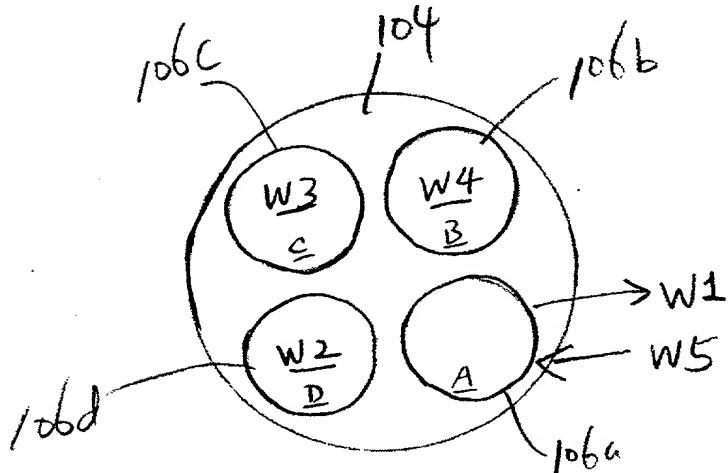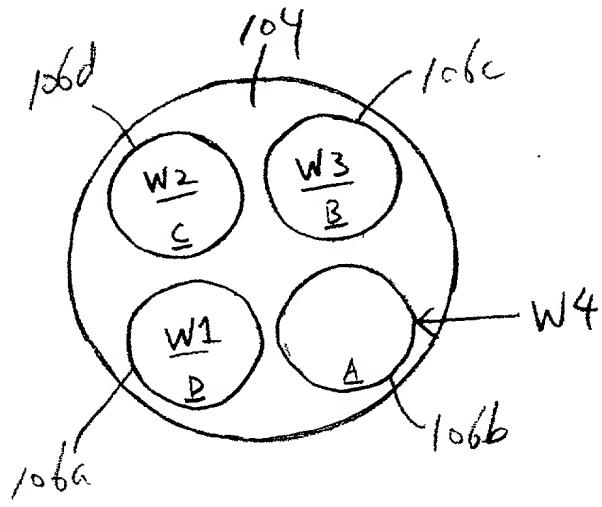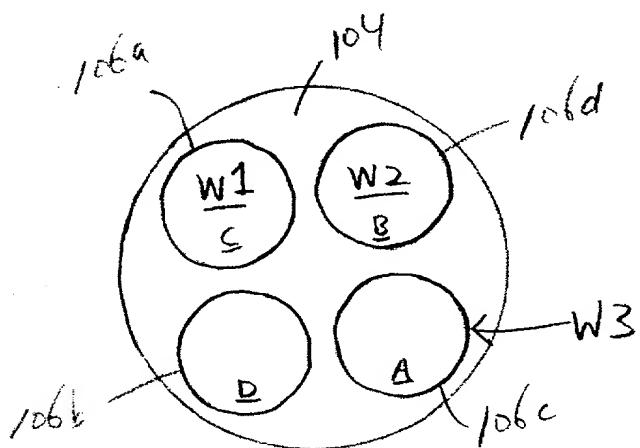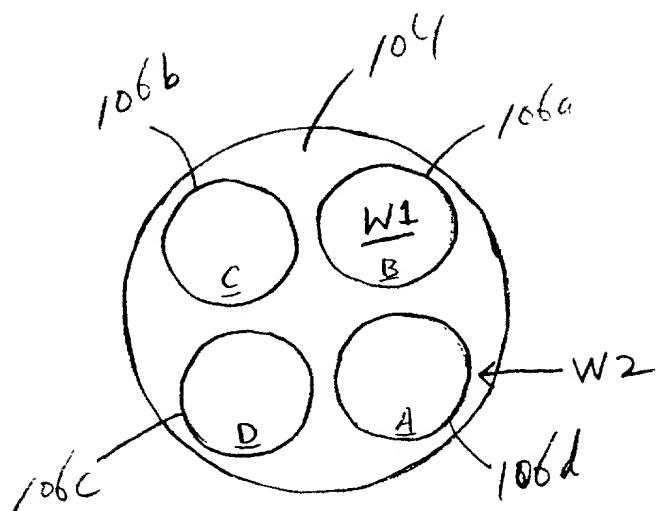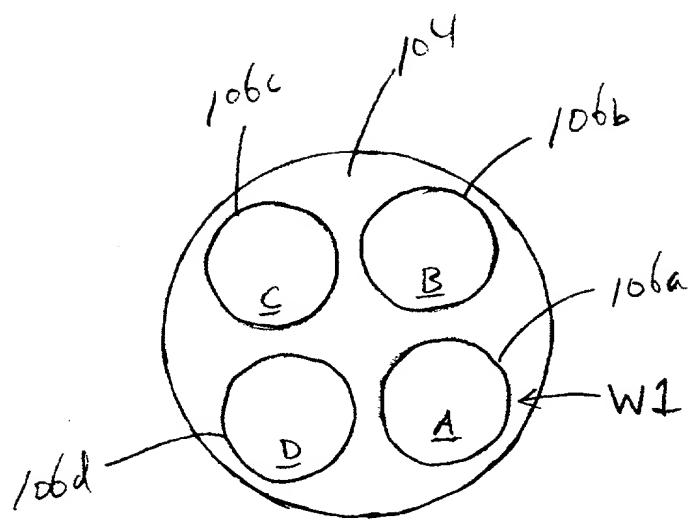

ORL-063

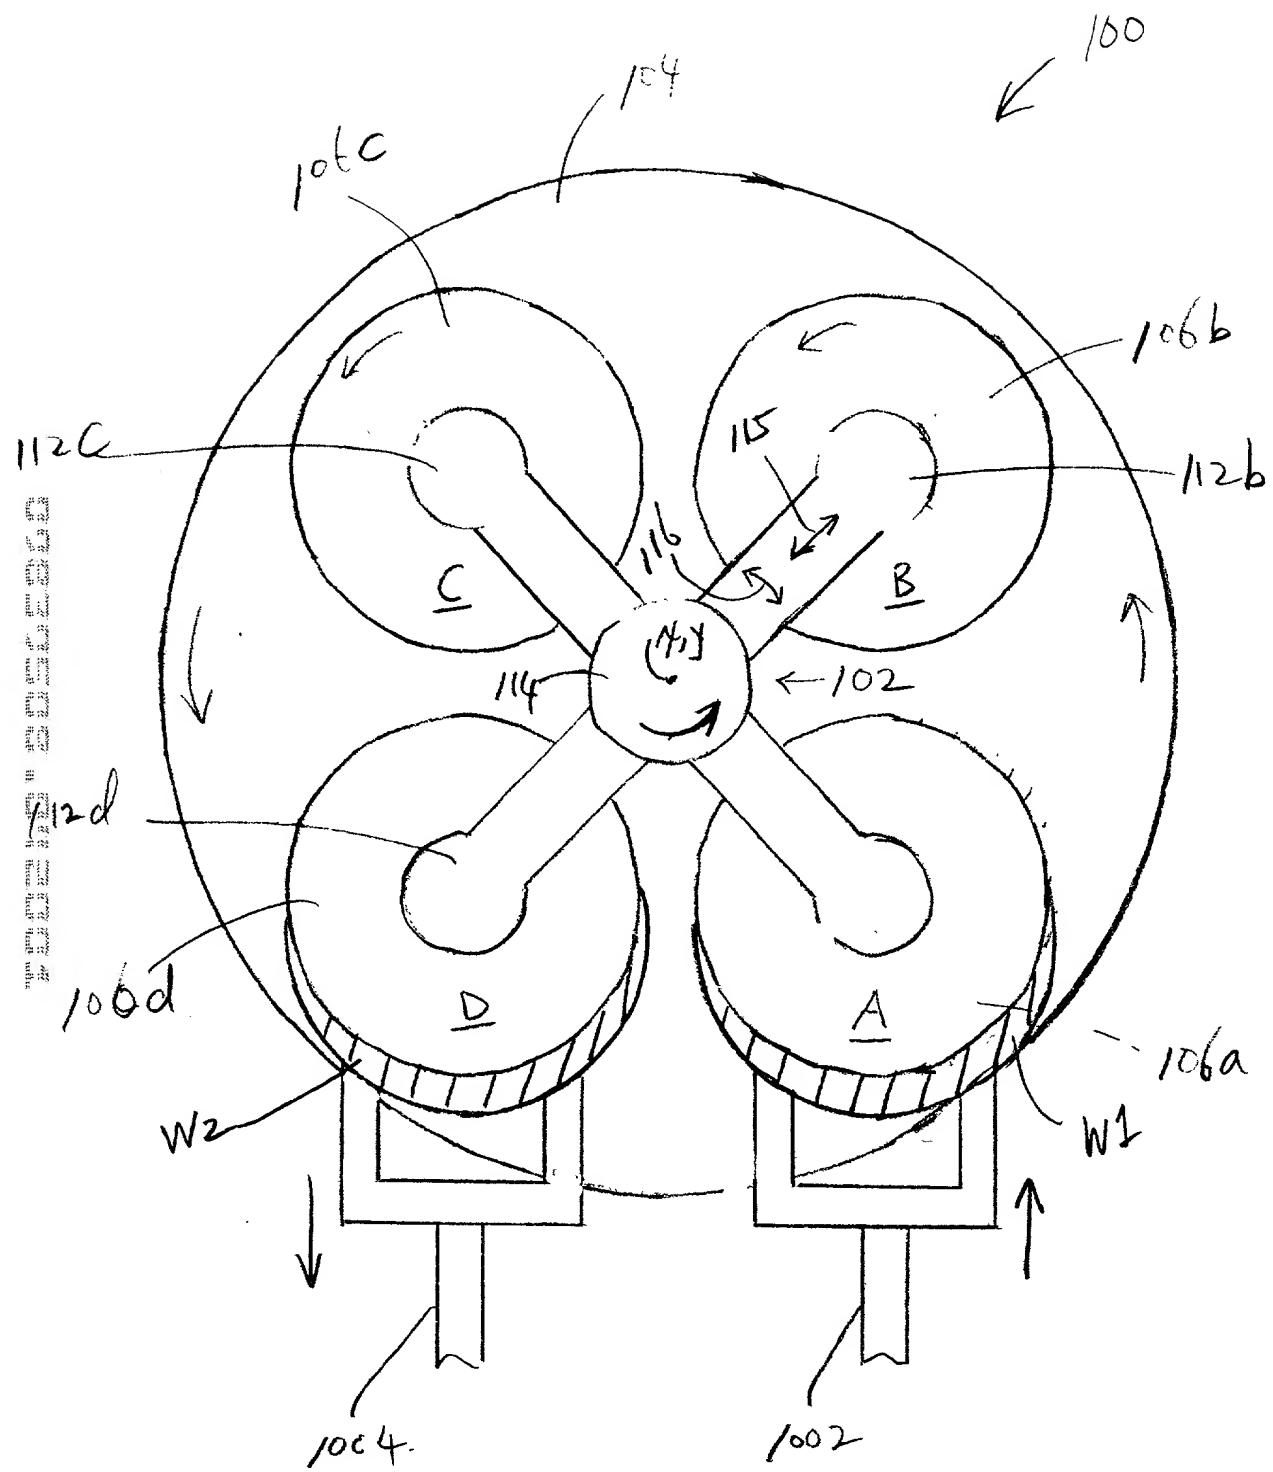


FIG. 10

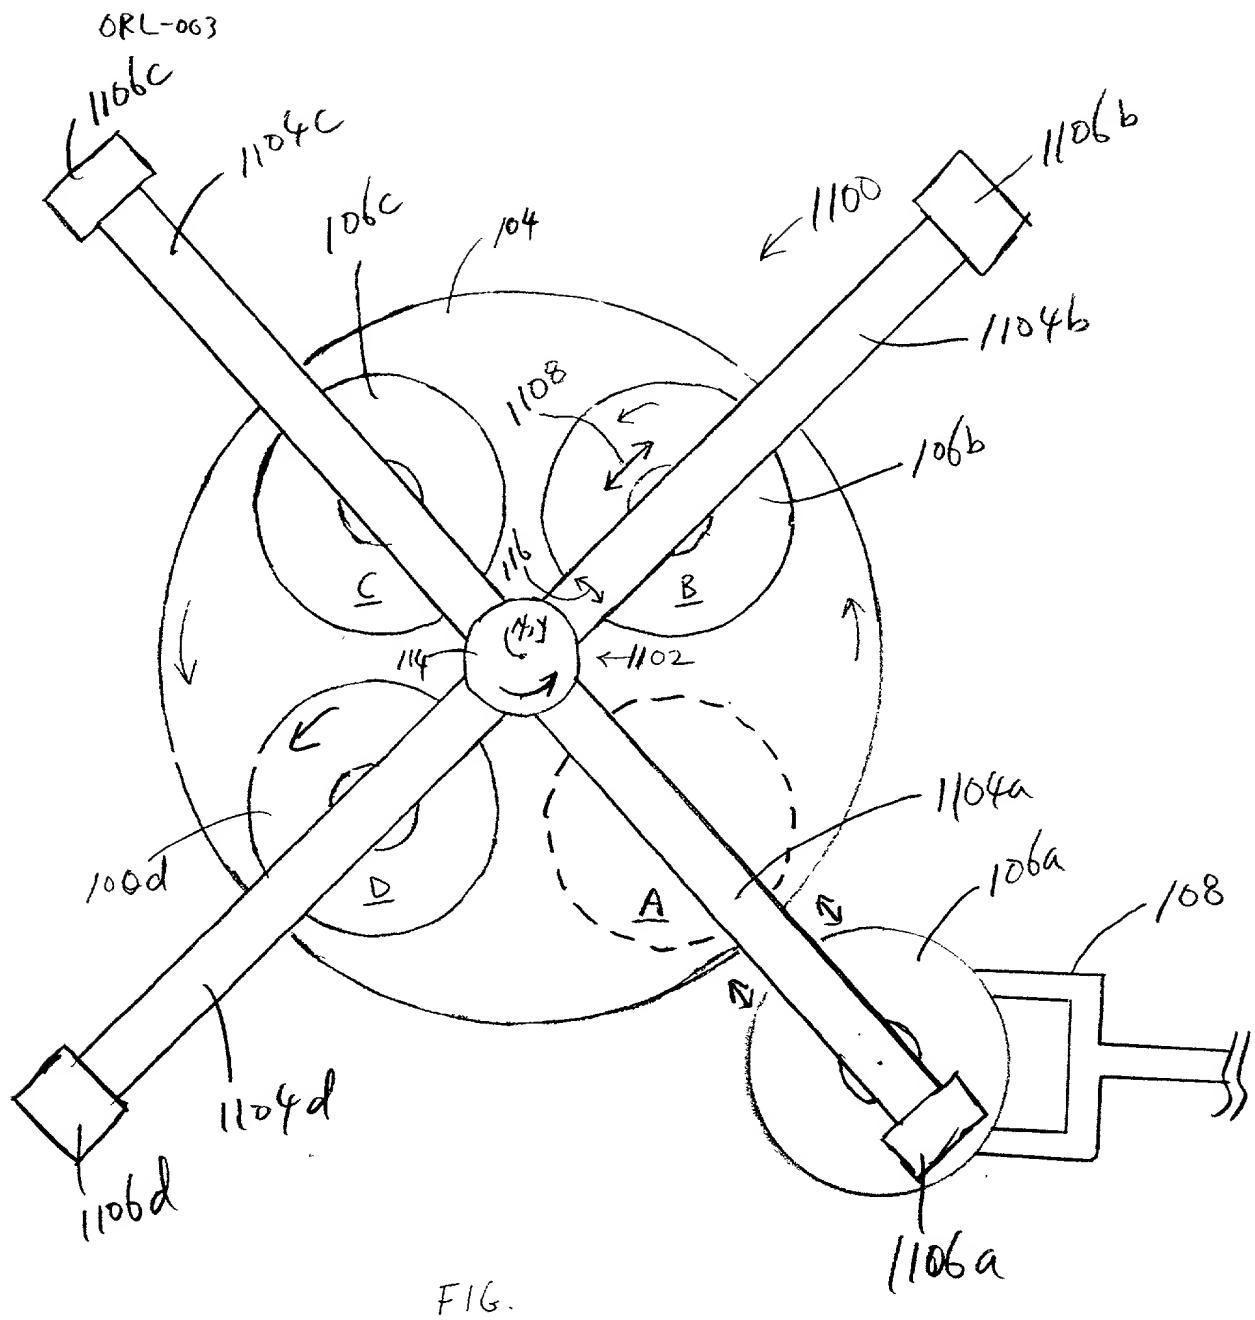
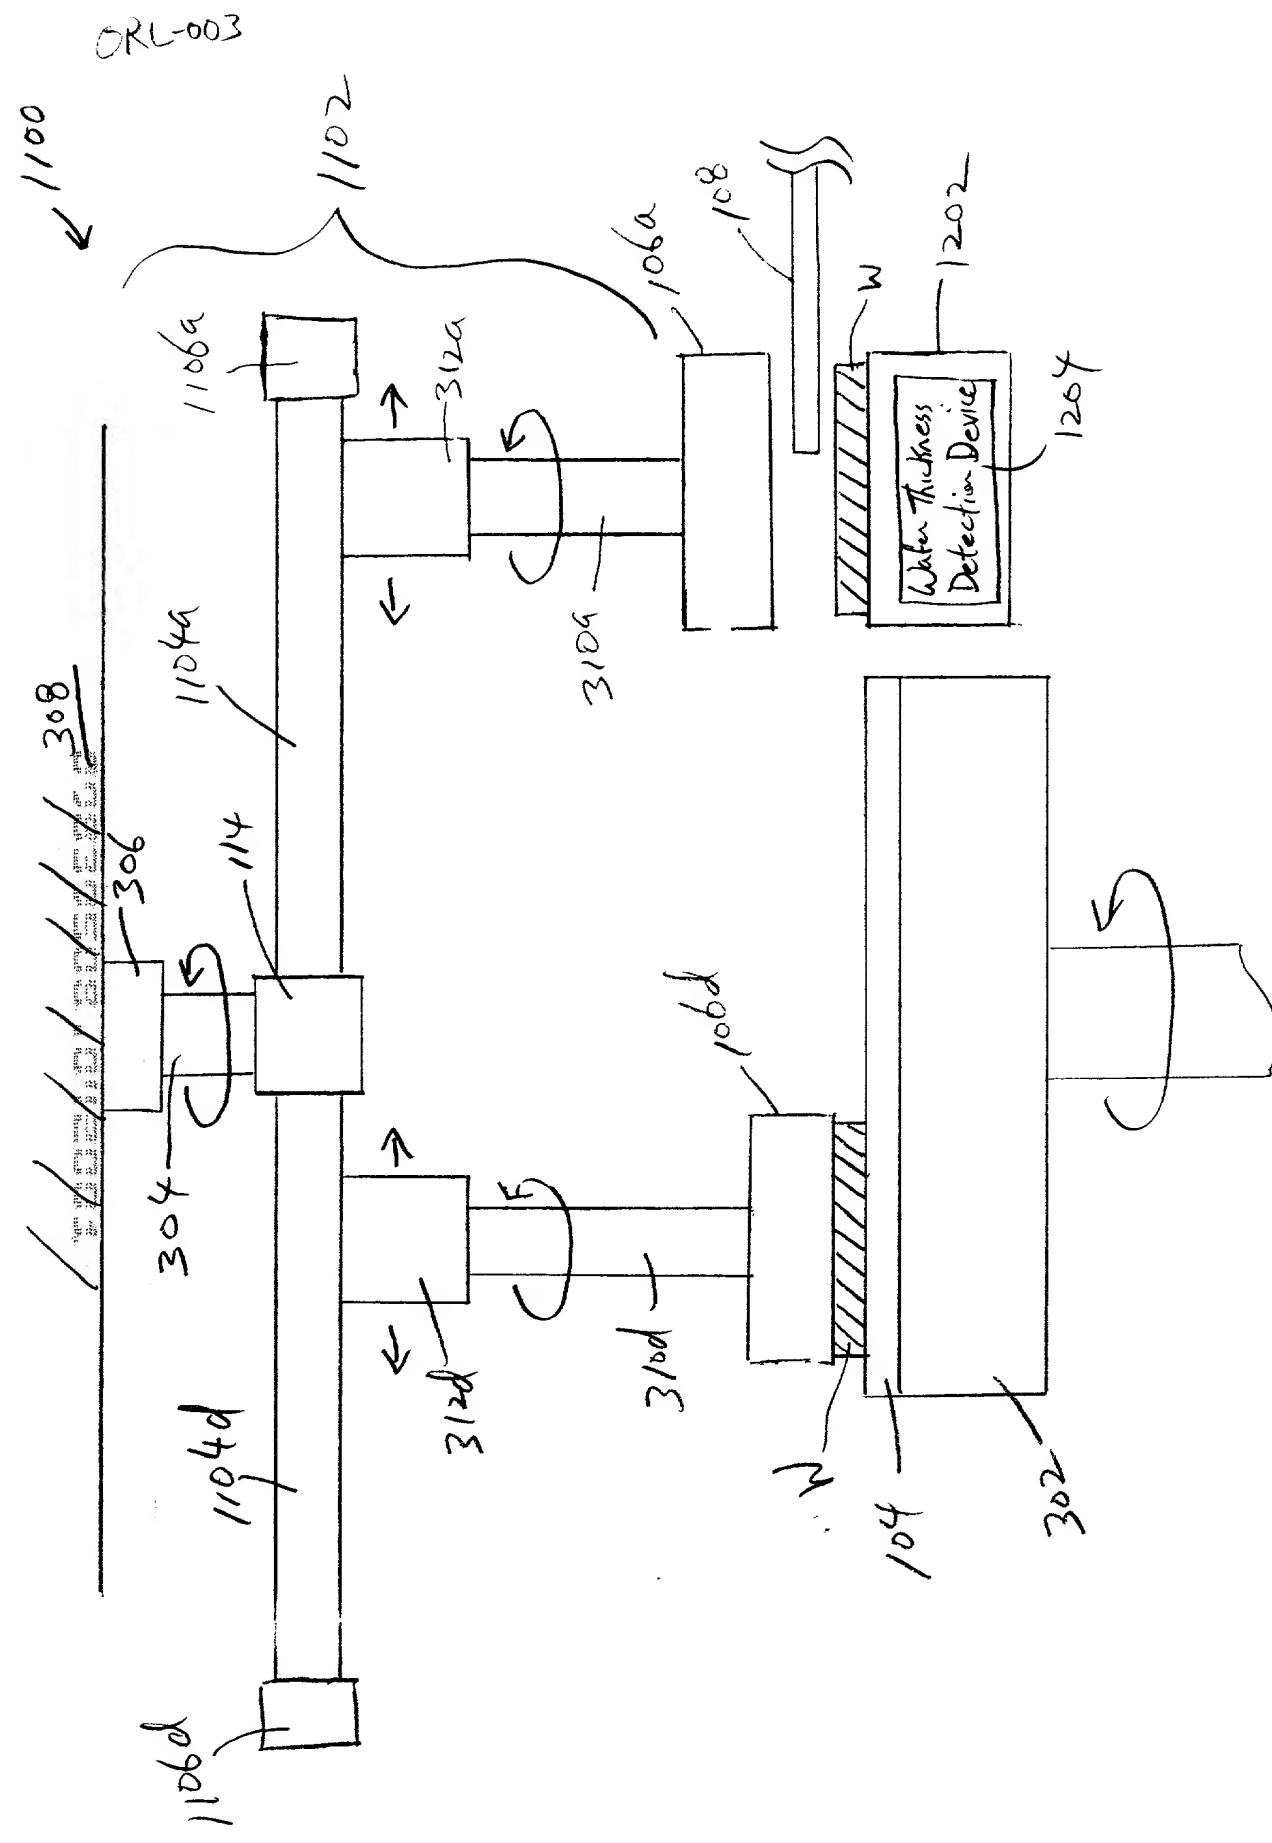


FIG. 11

FIG. 12



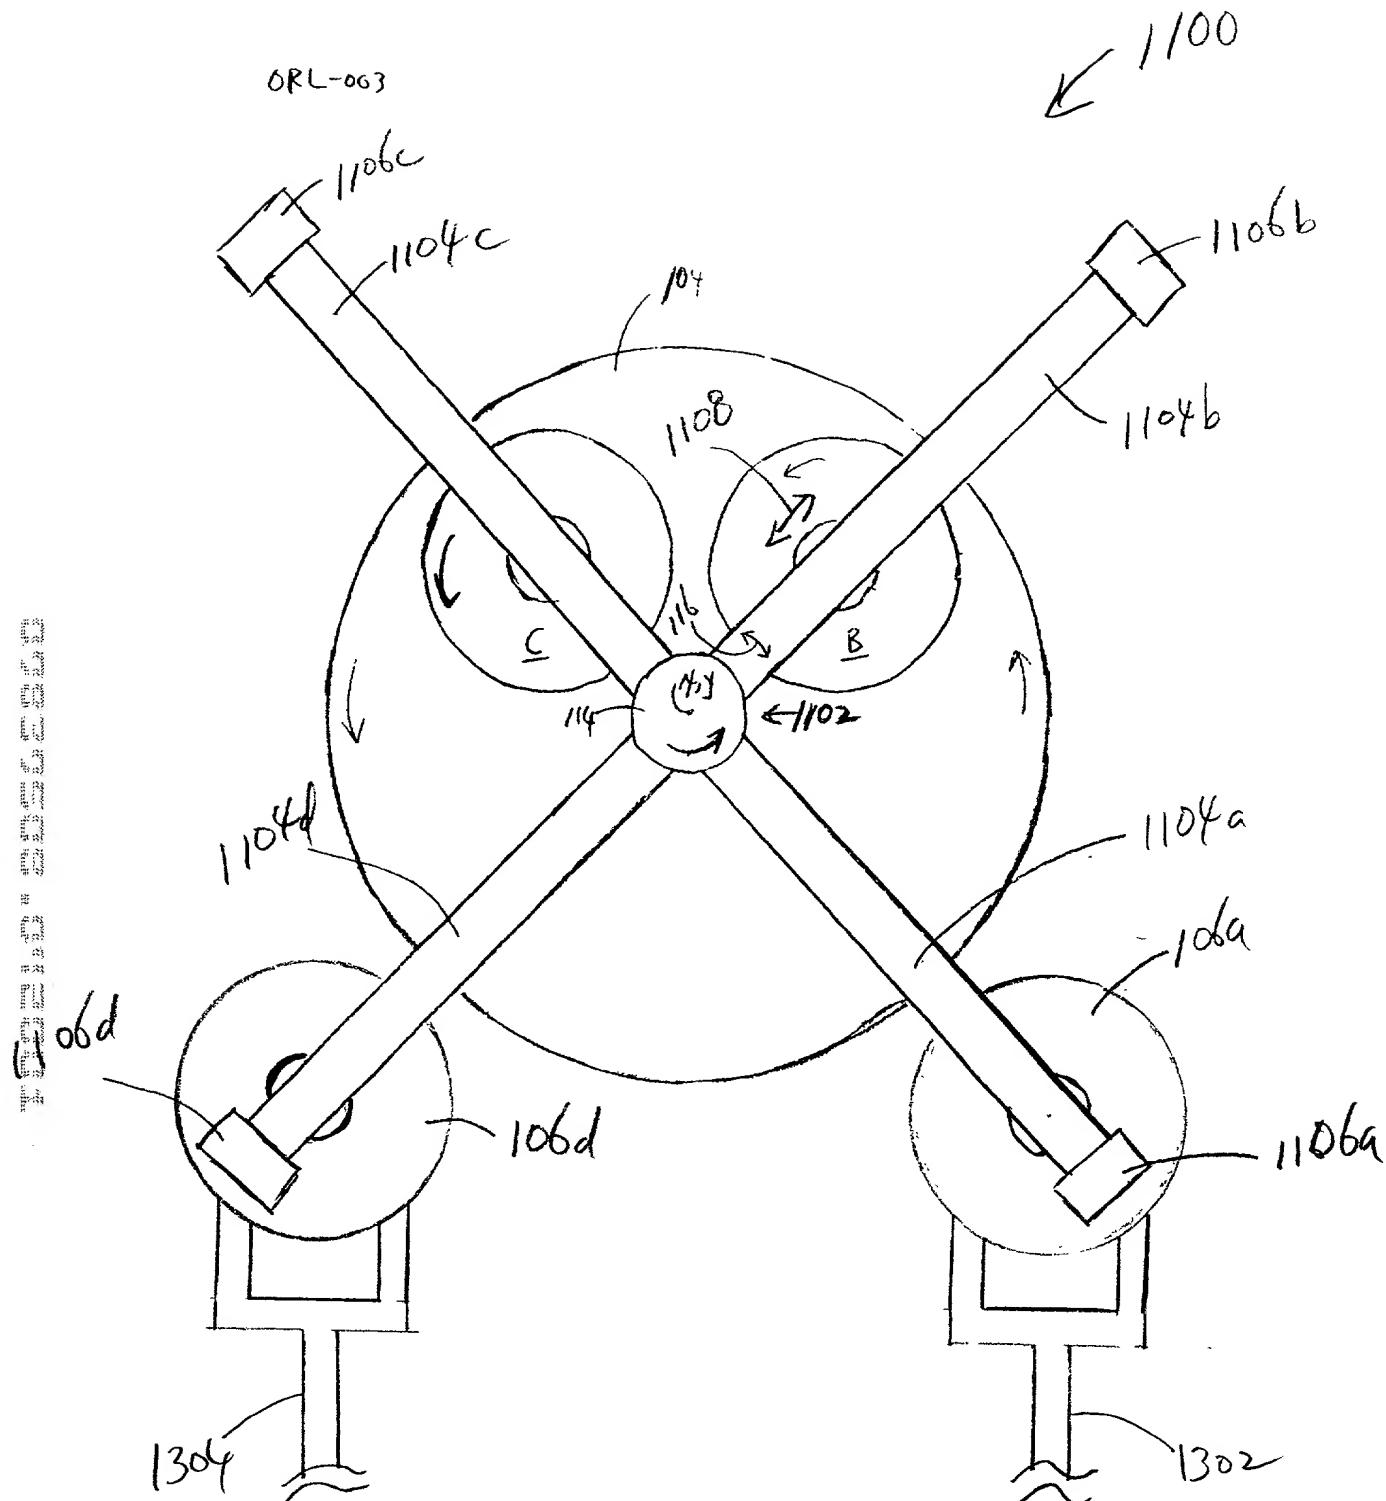


FIG. 13

ORL-003

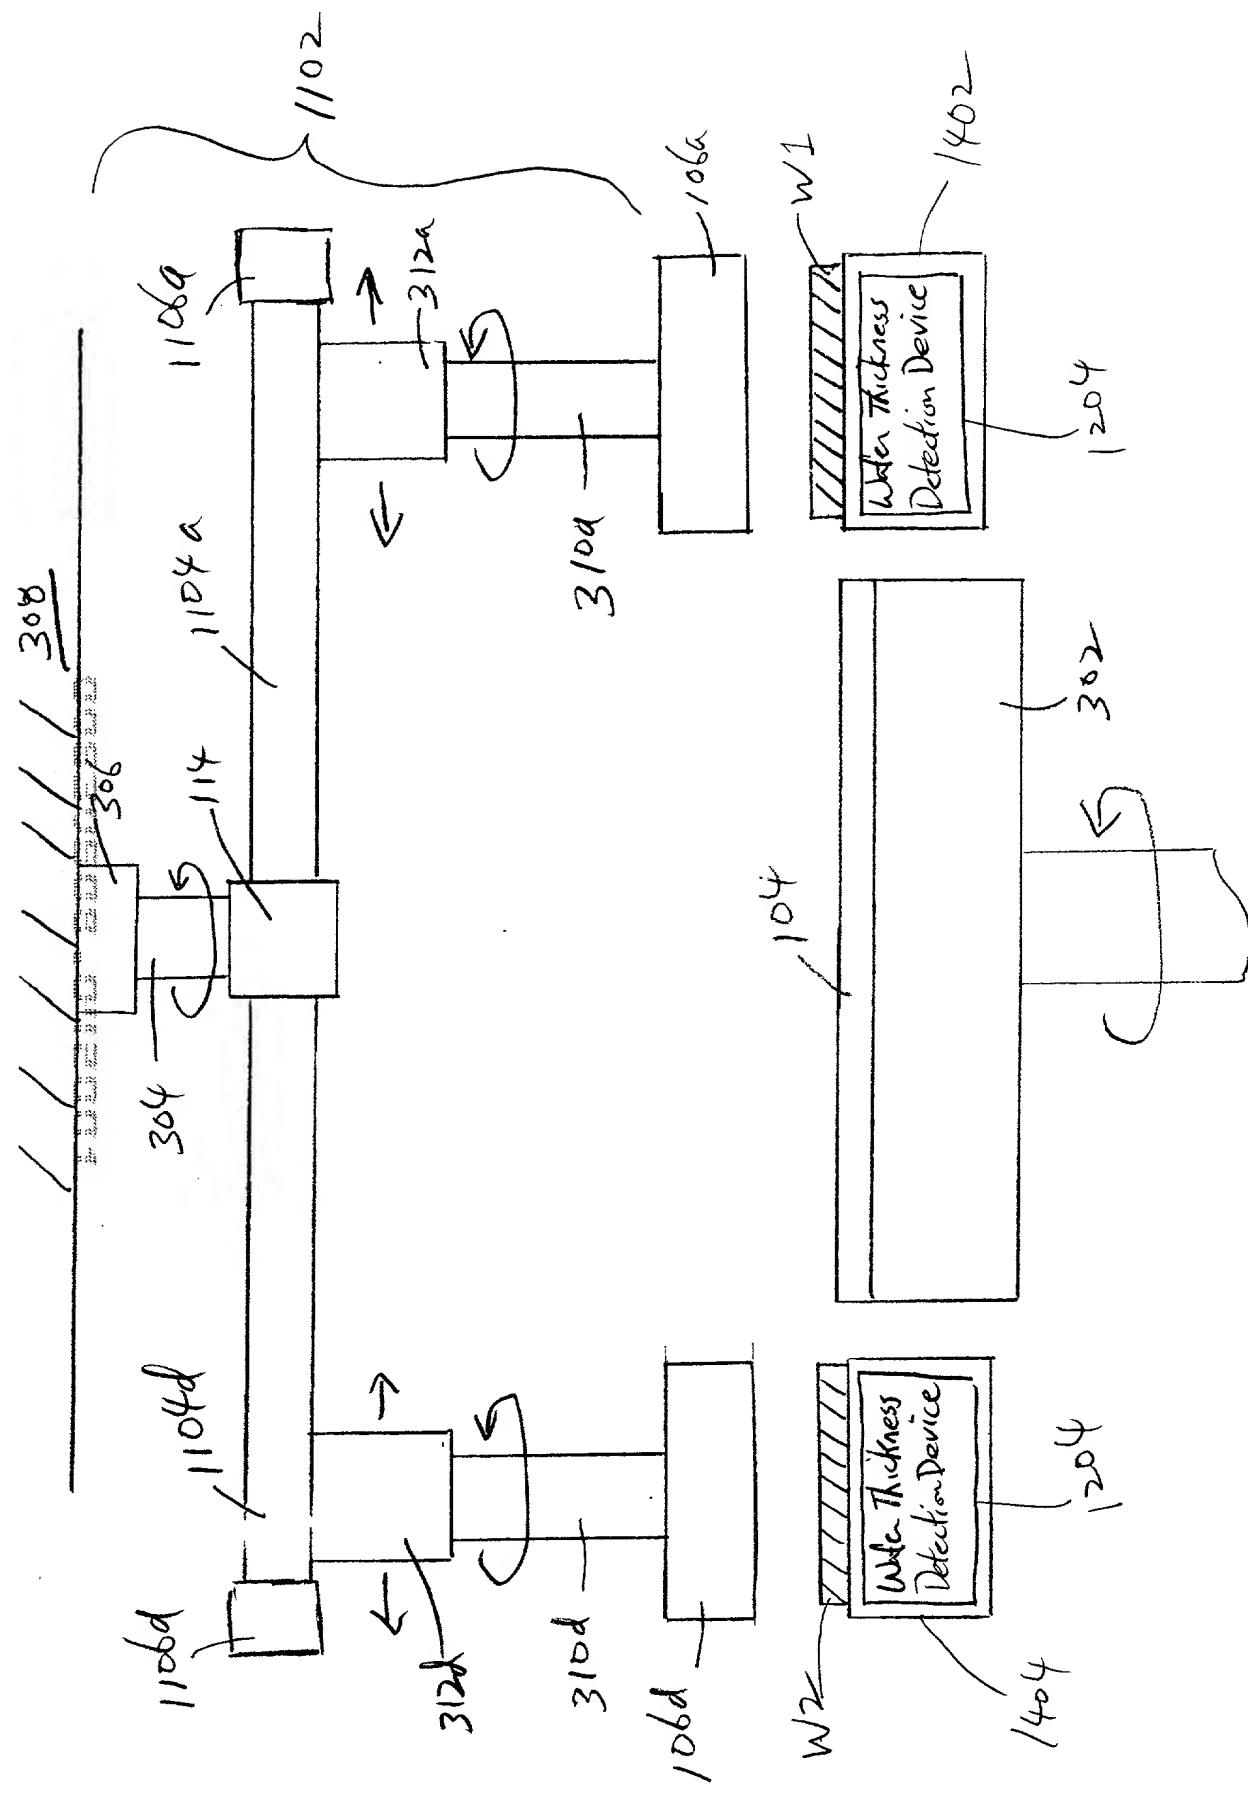


FIG. 14

6RL-003

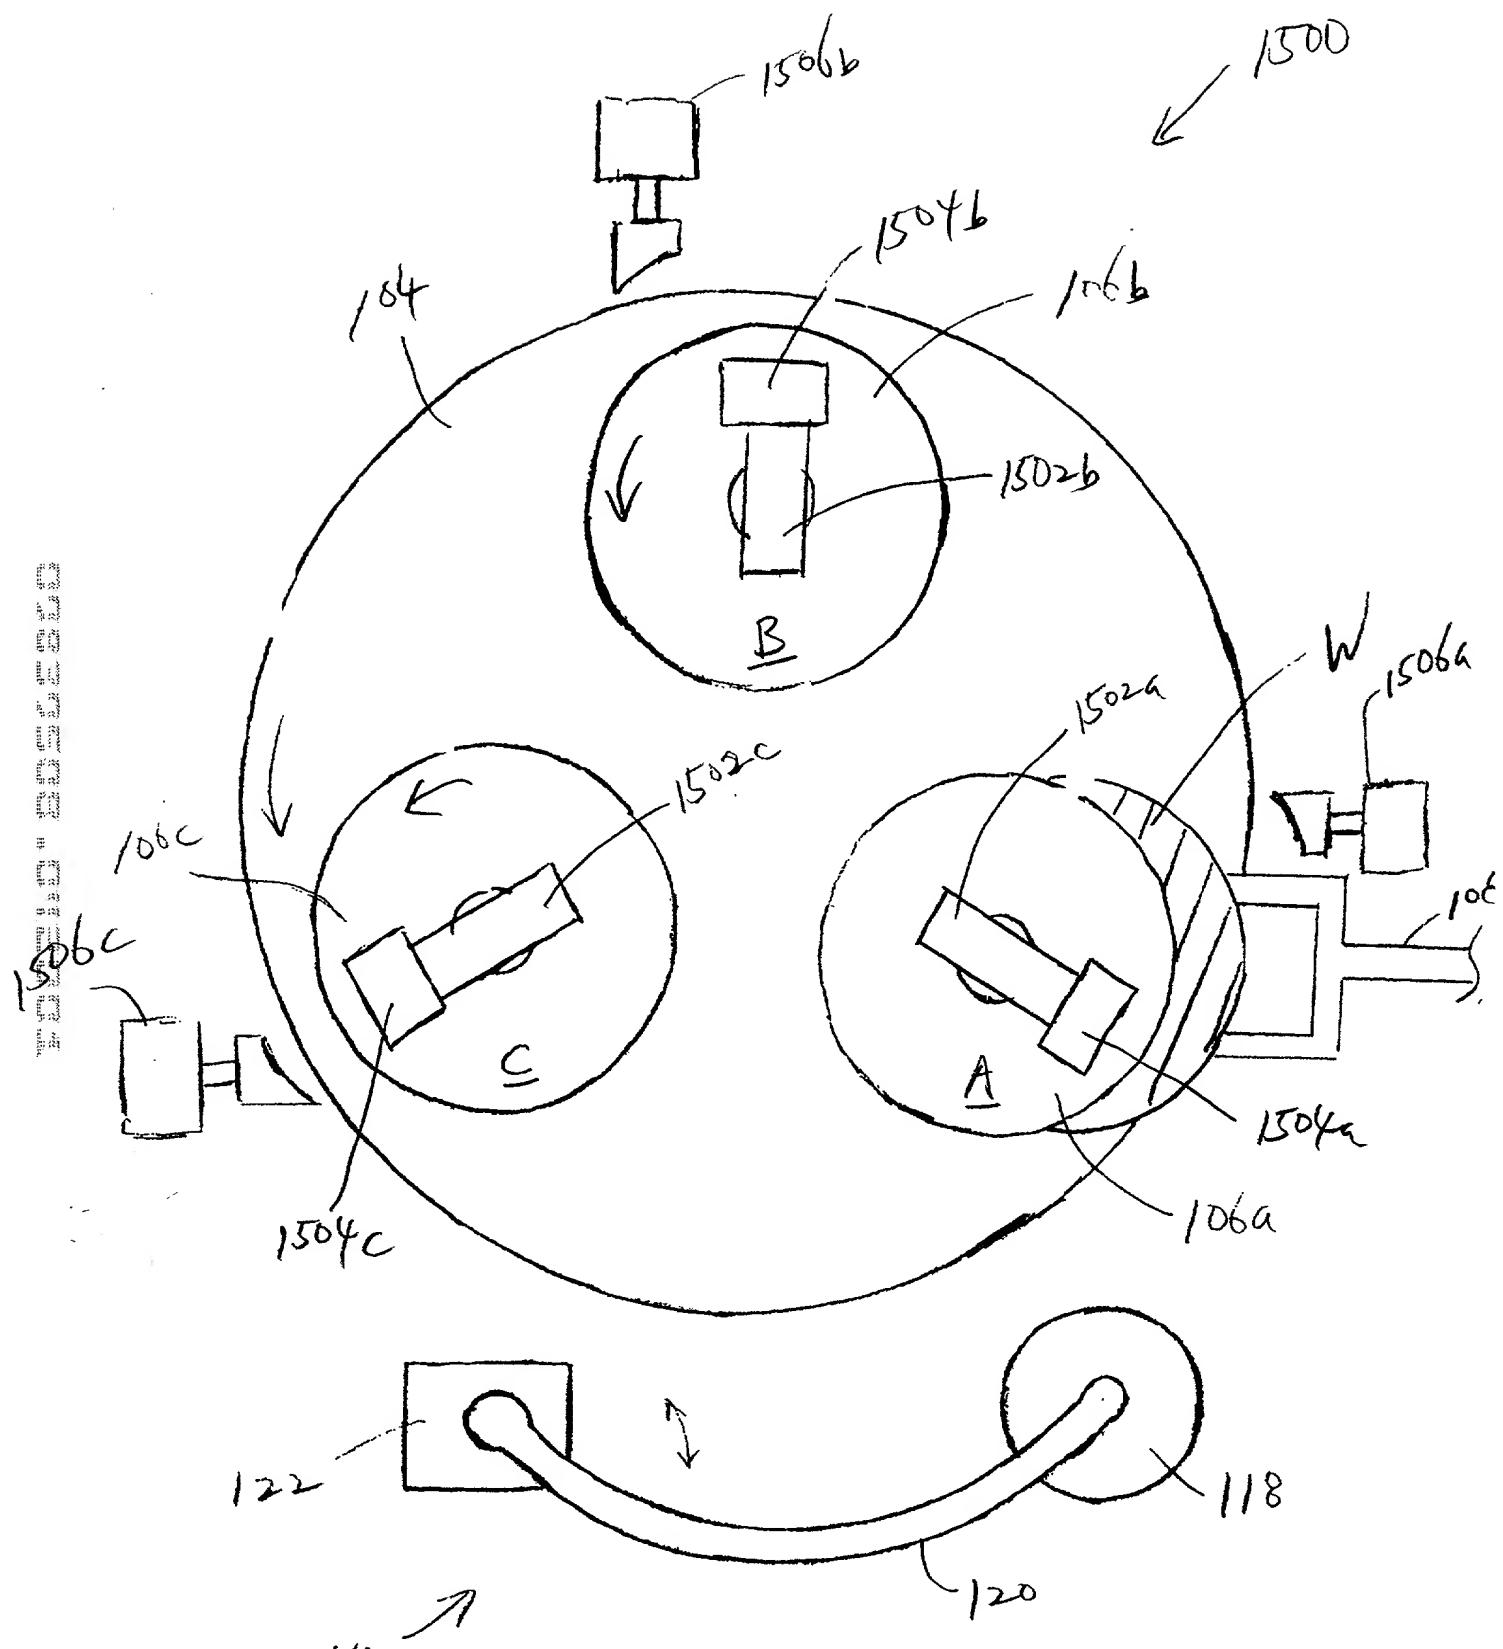


FIG. 15

OFL-063

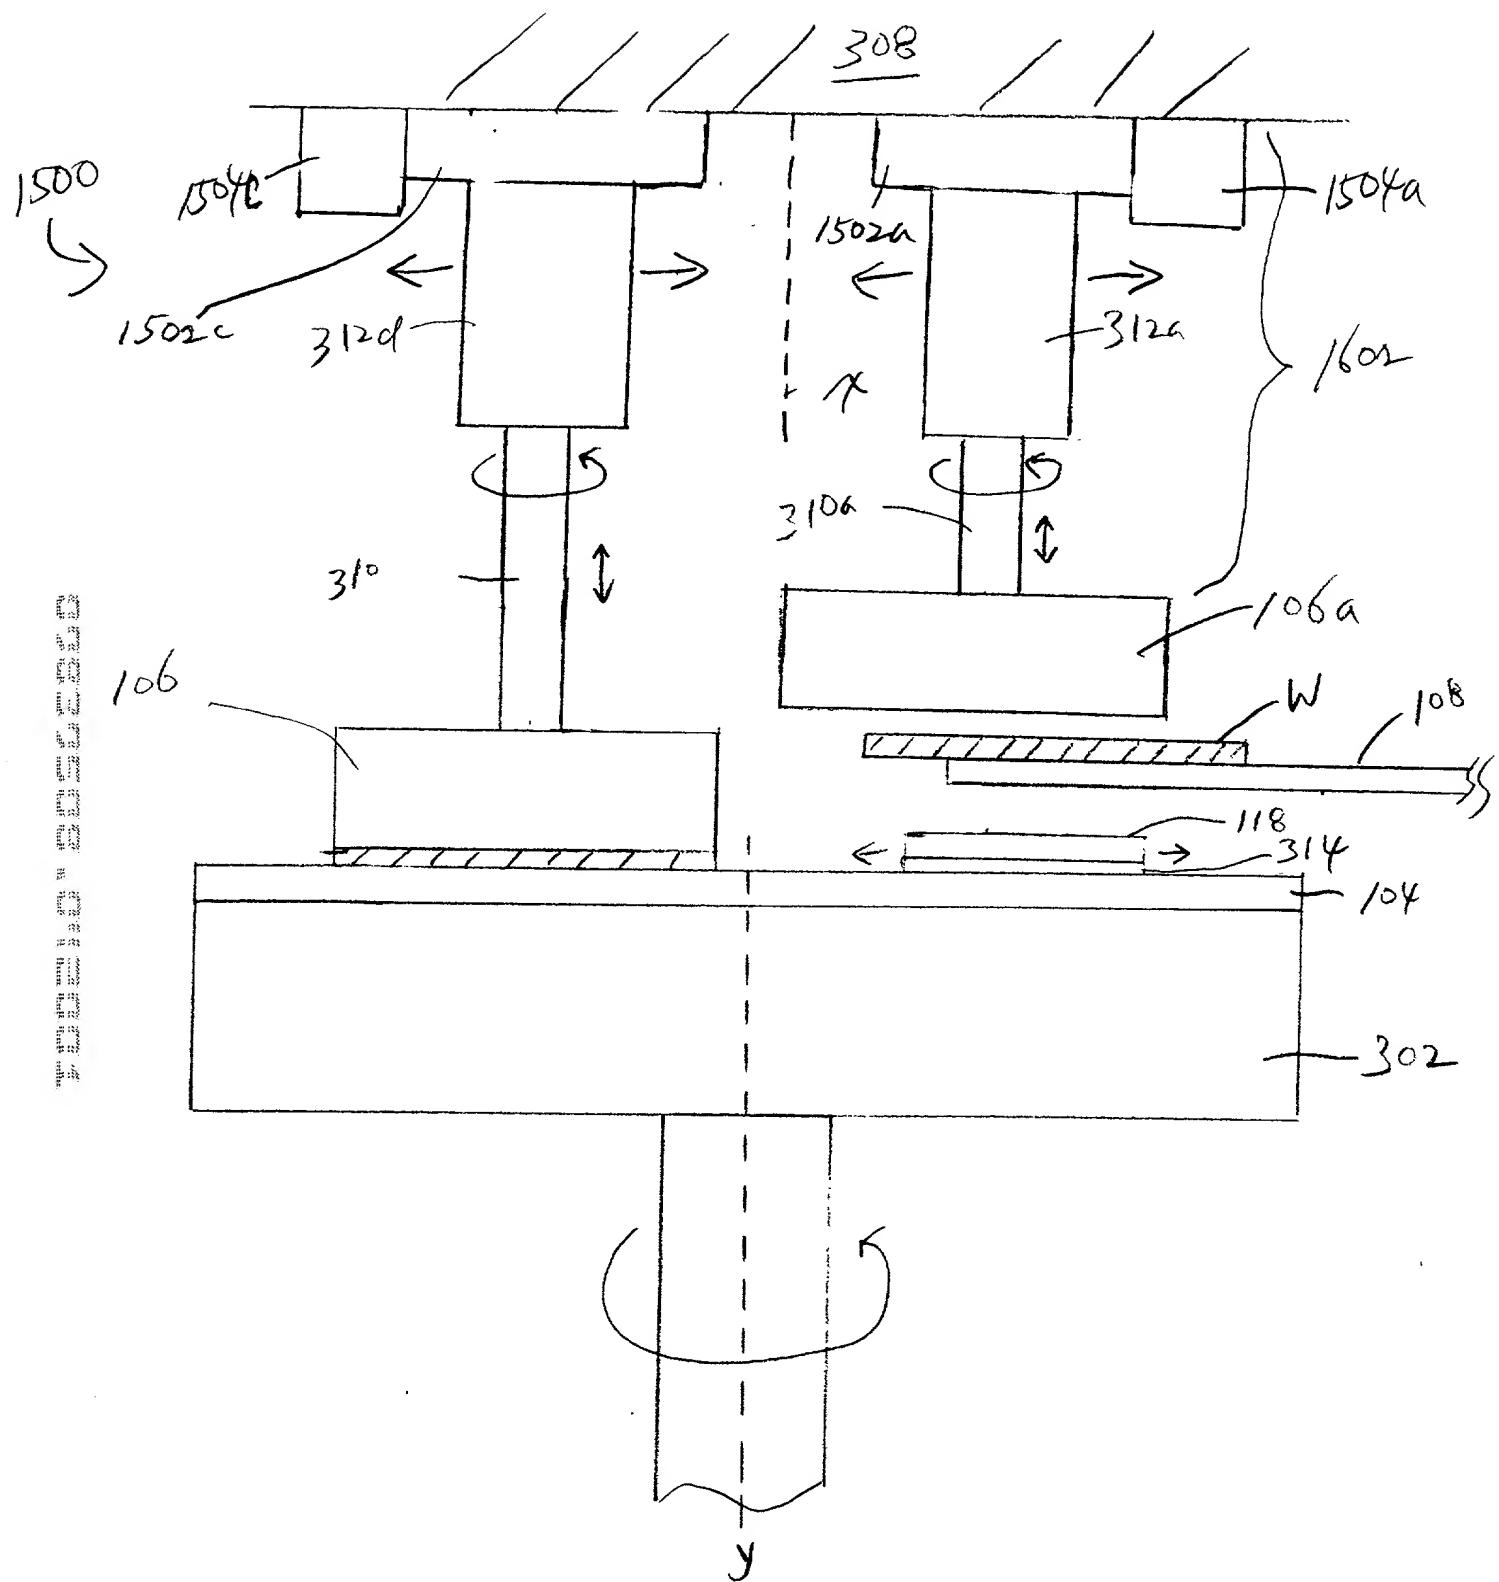


FIG. 1b

ORC-003


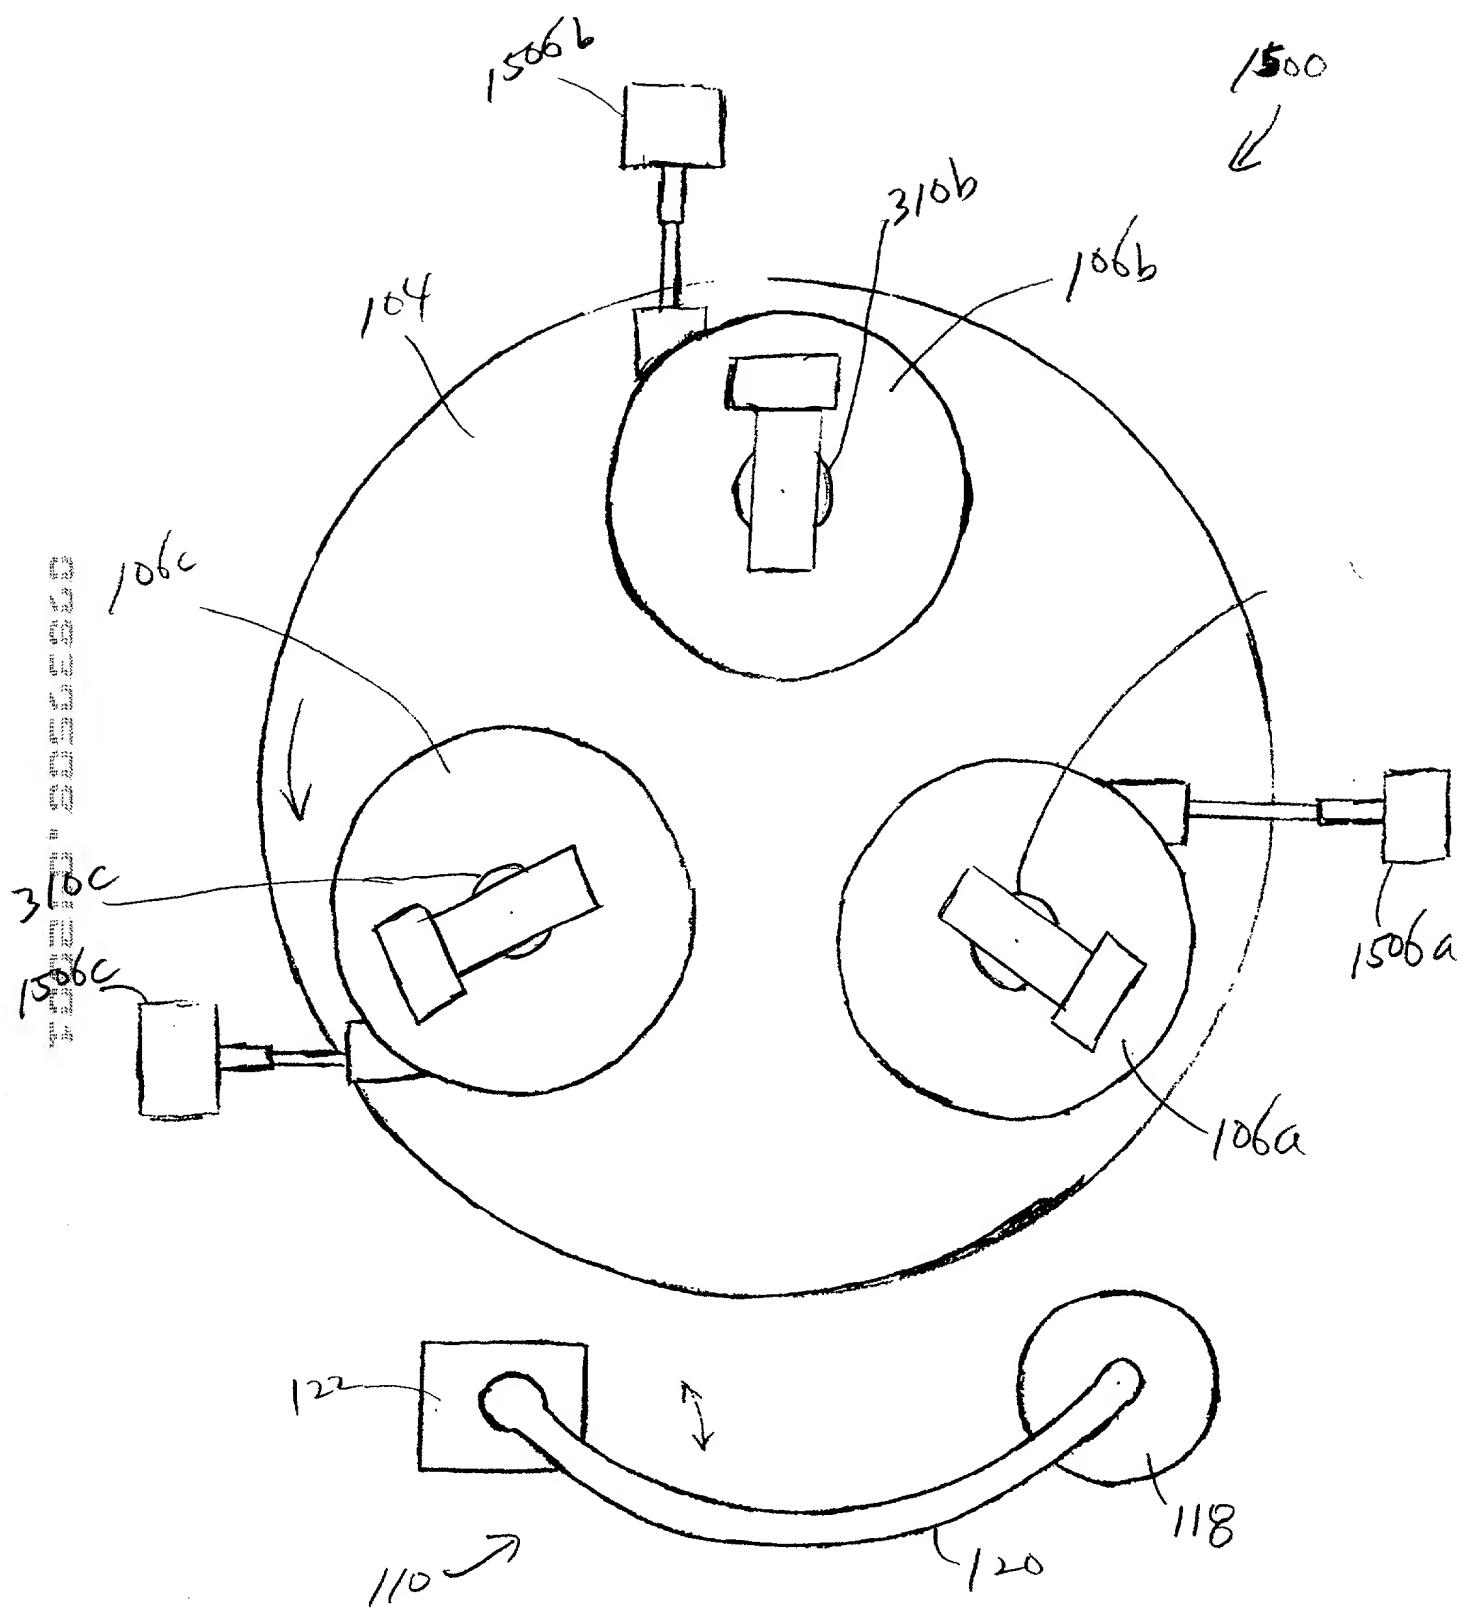


FIG. 17

ORL-003

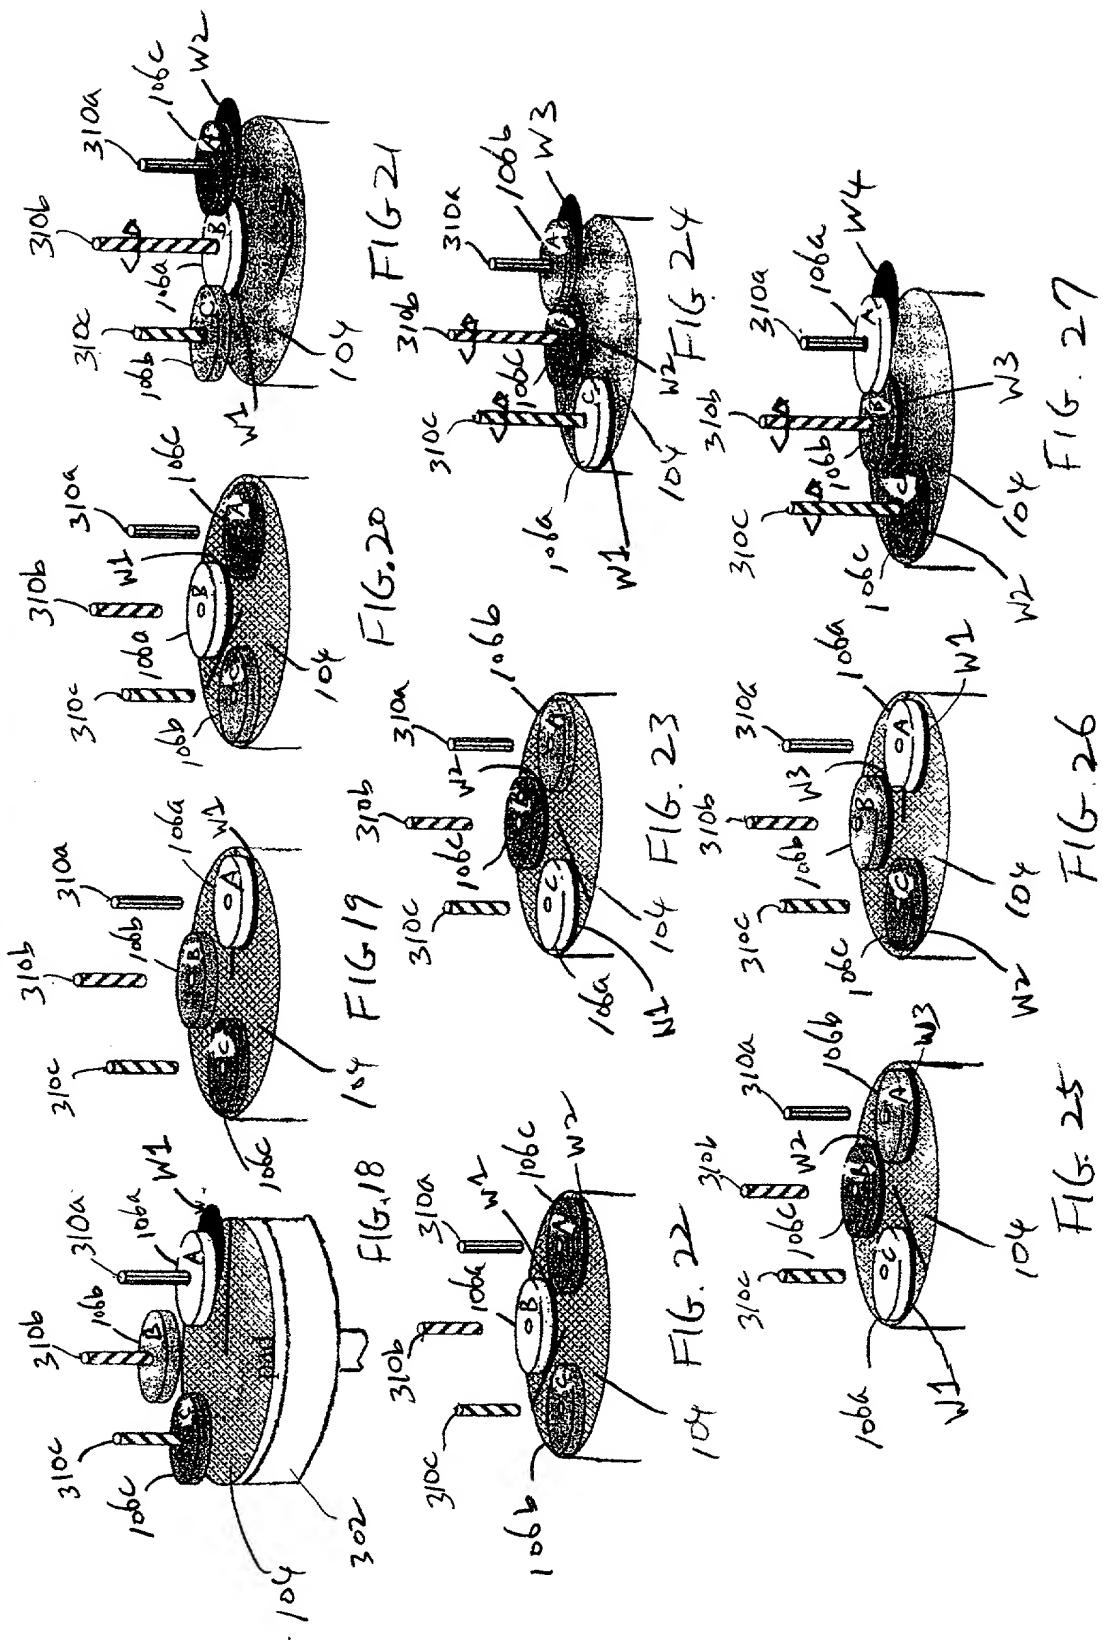

ORL-003

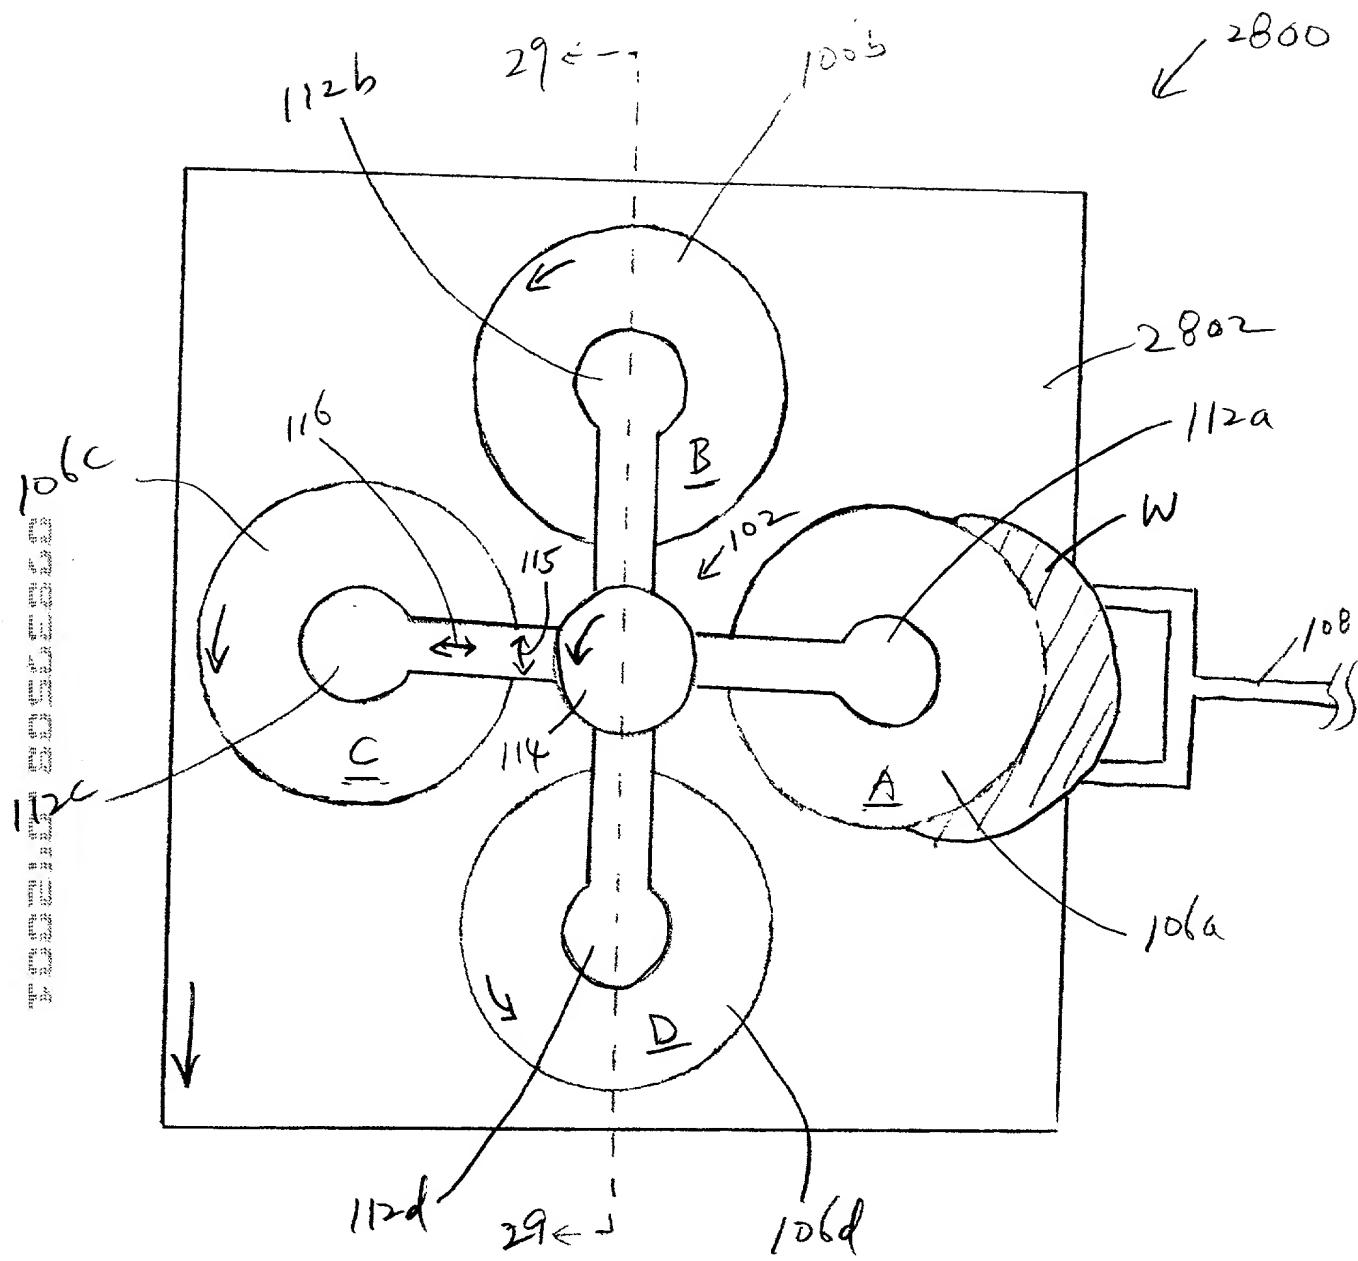


FIG. 28

ORL-003

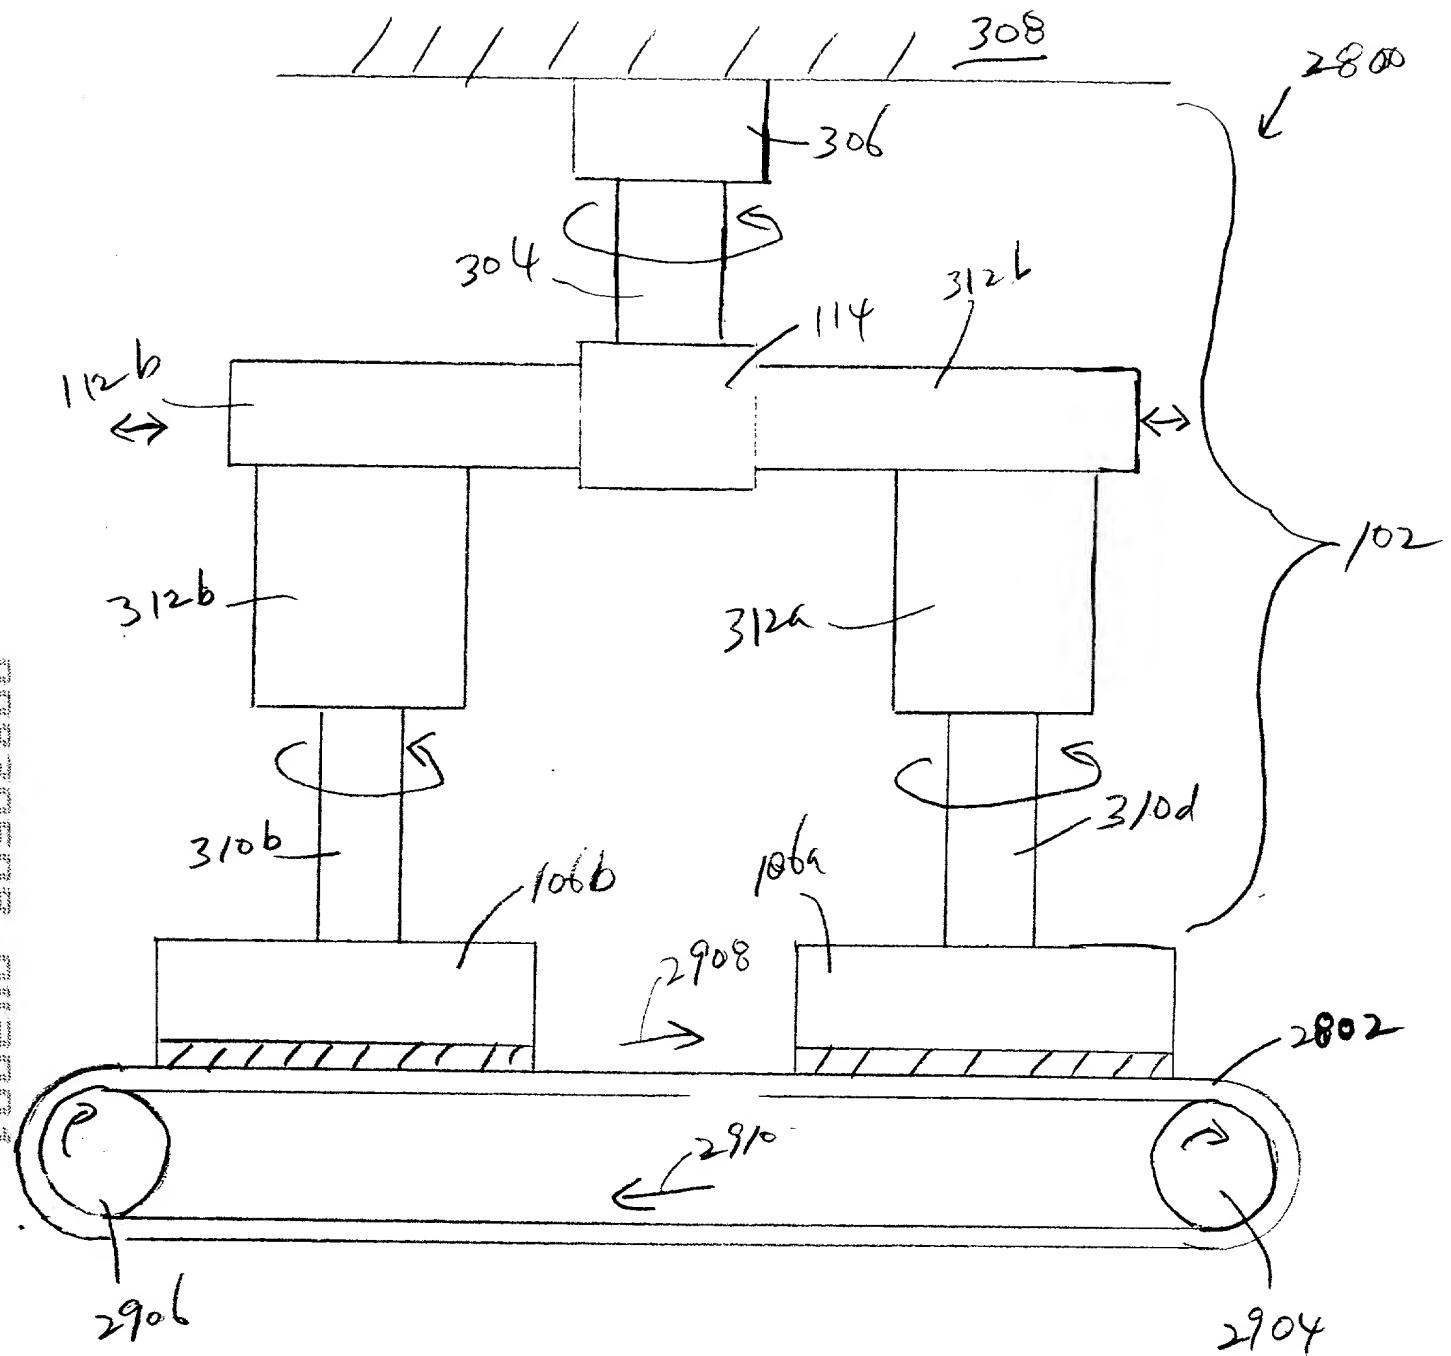


FIG. 29

ORL-003

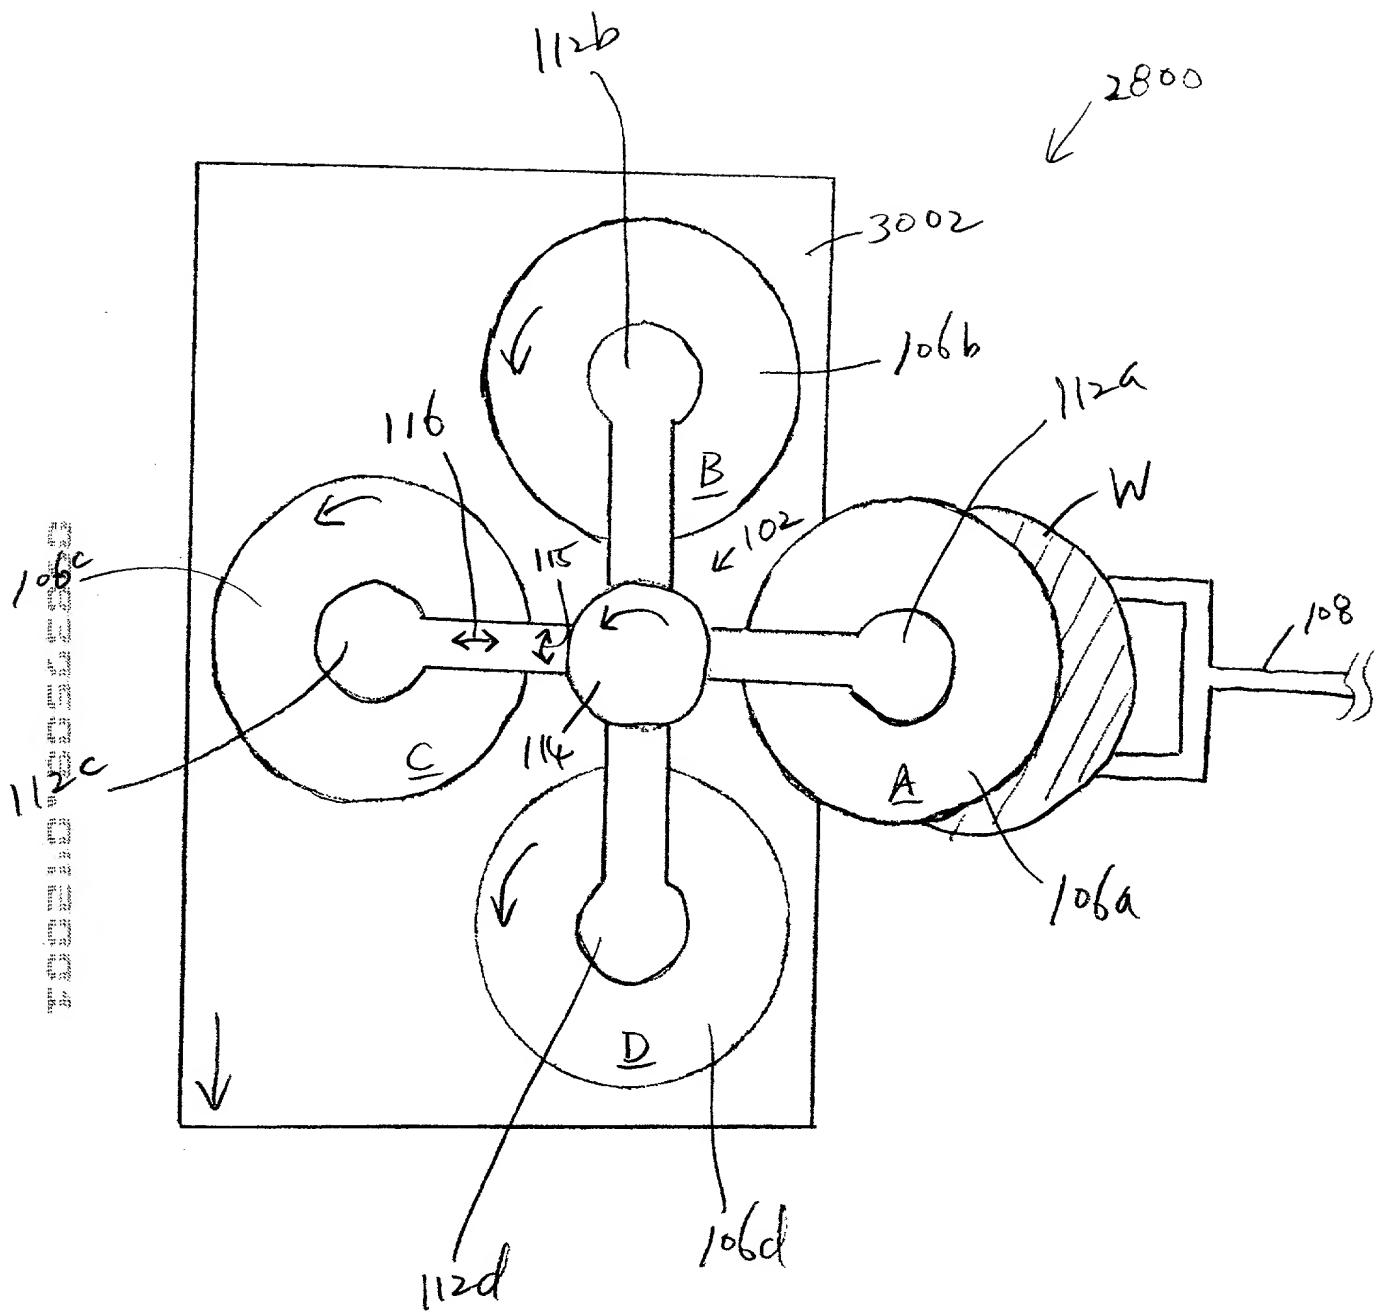


FIG. 30.



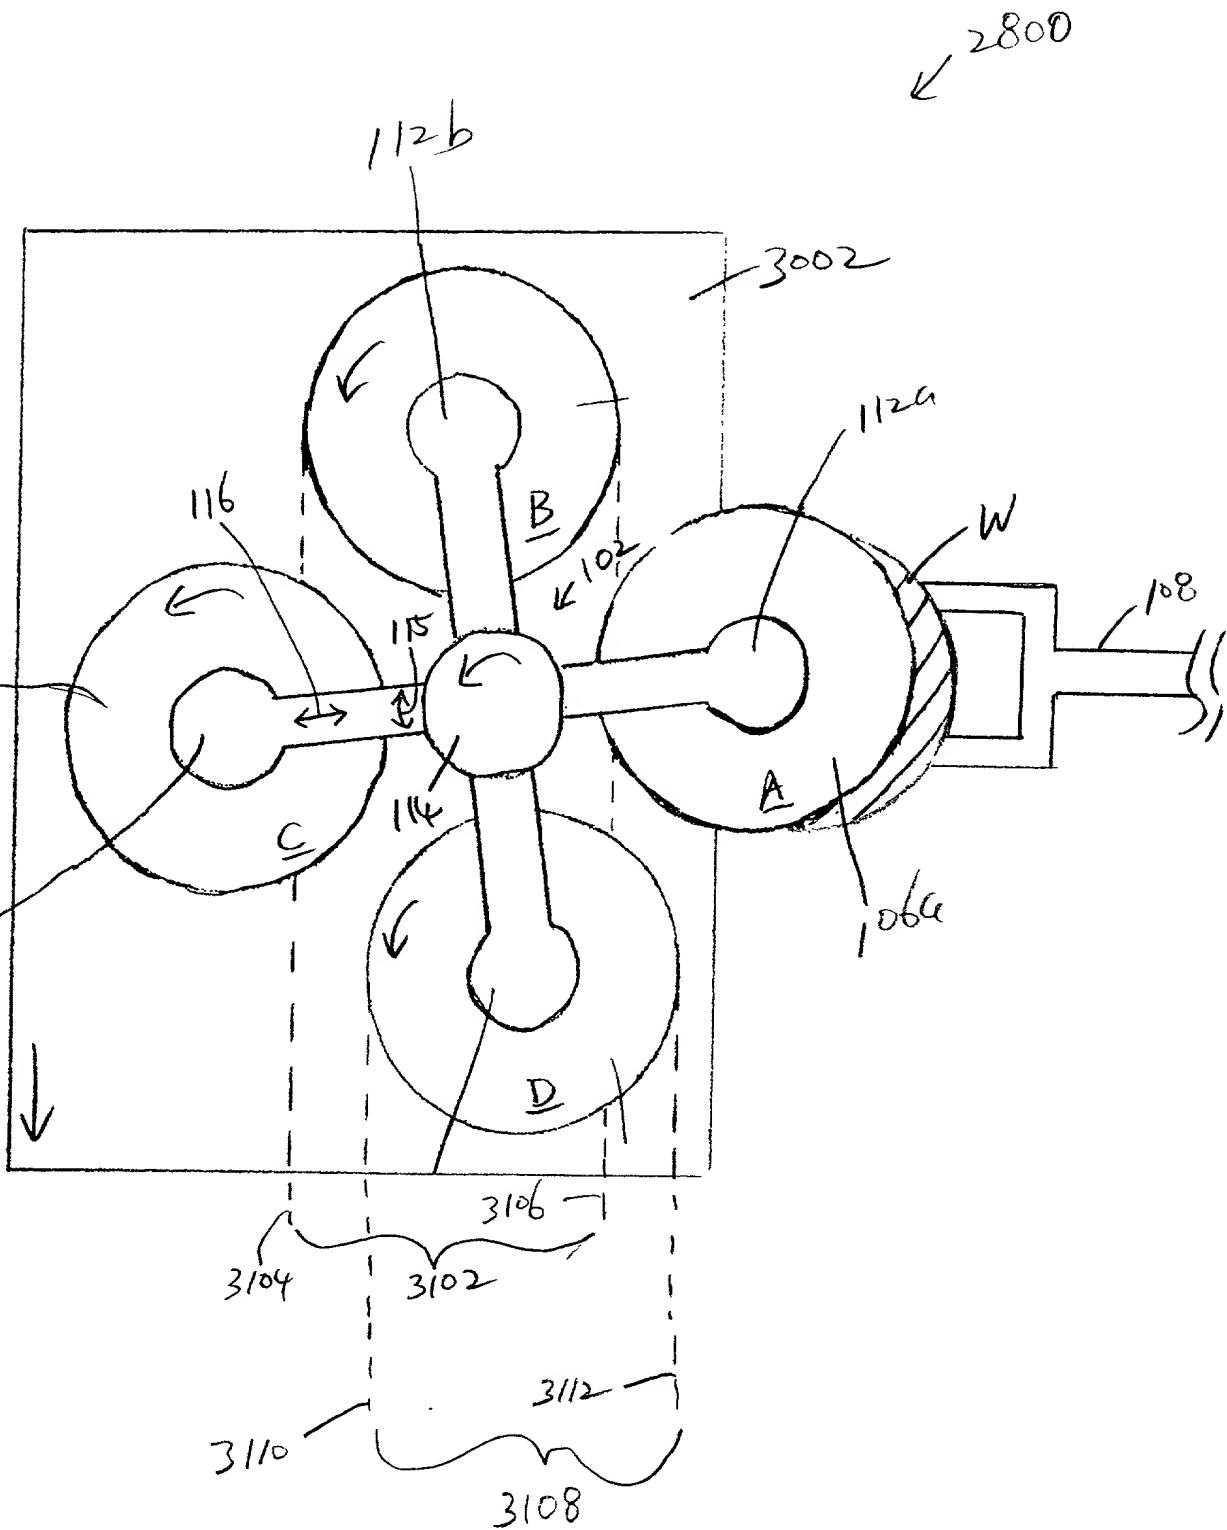


FIG. 31

6RL-003

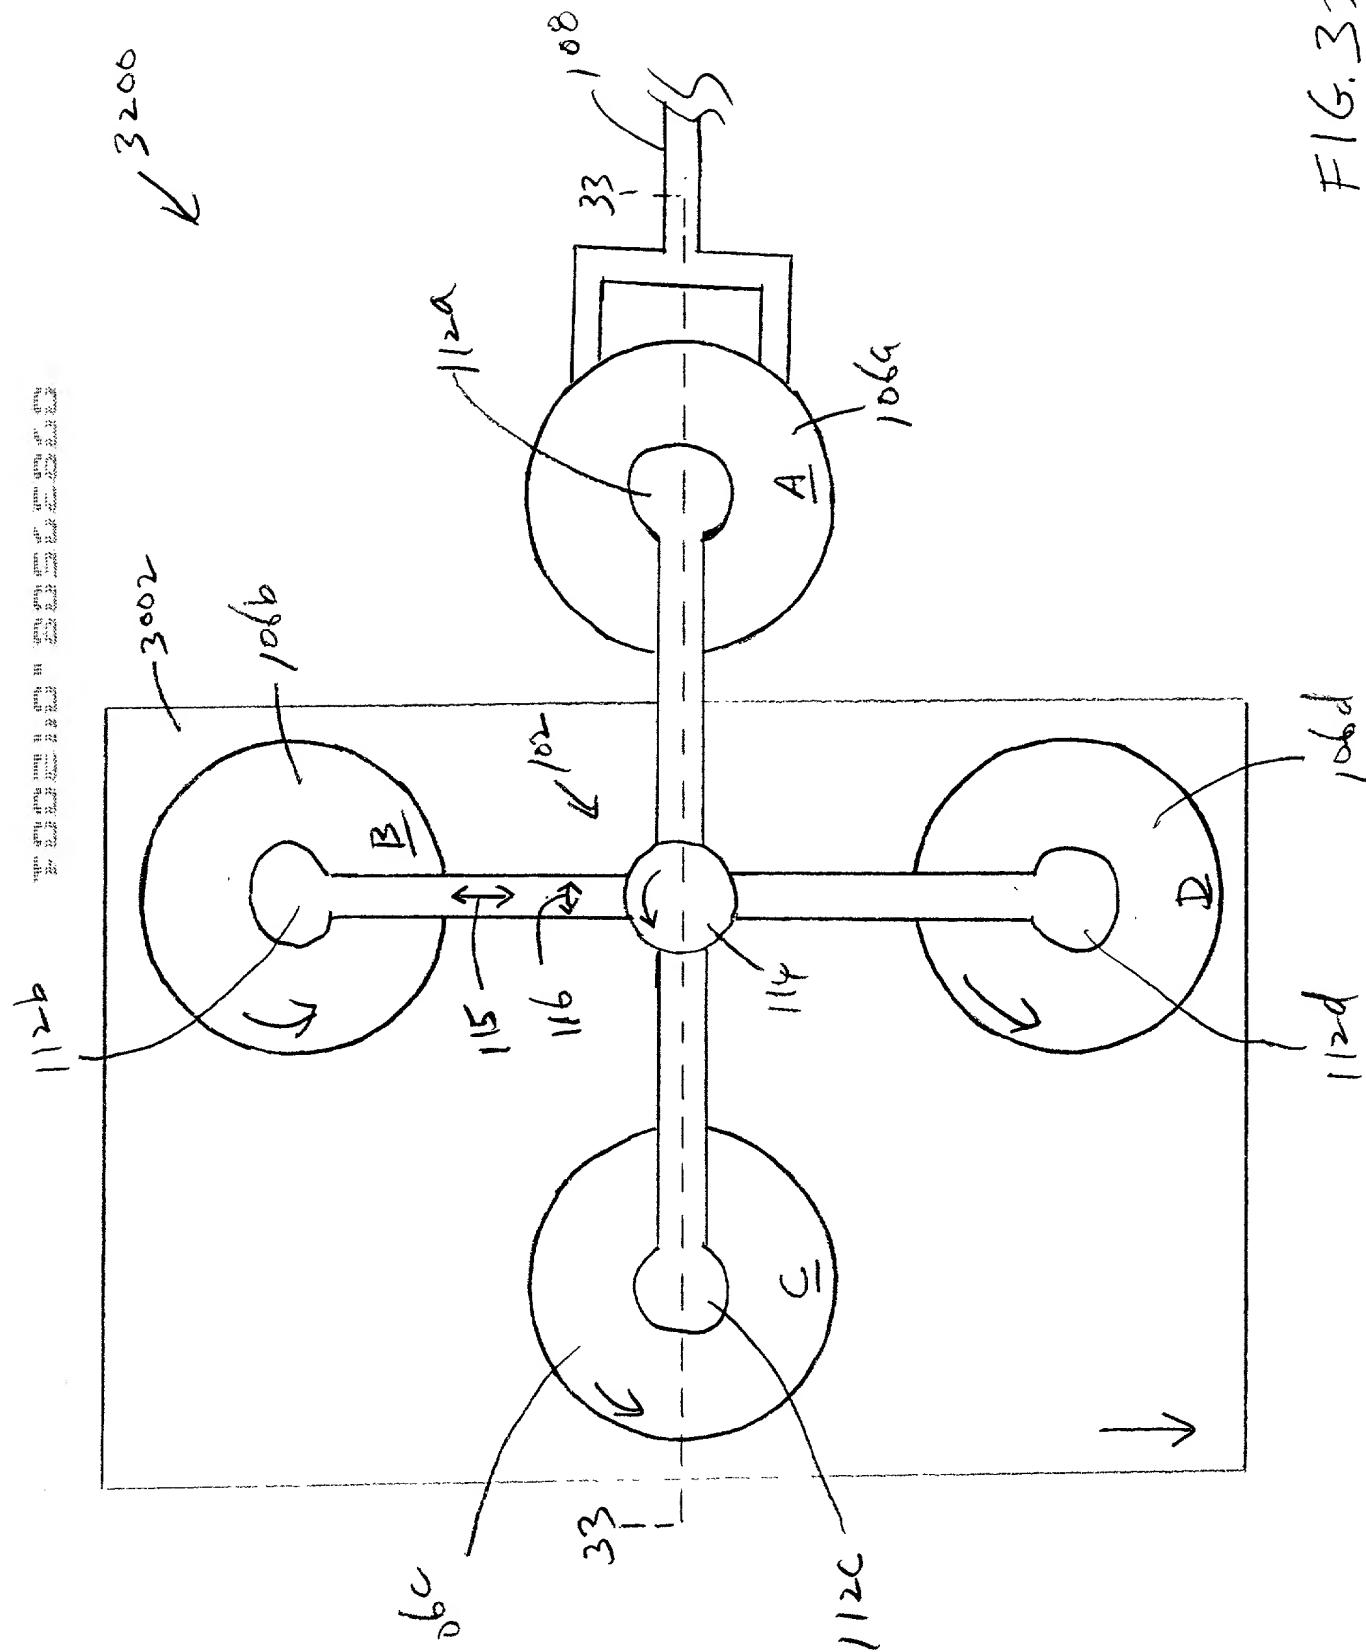

ORL-003


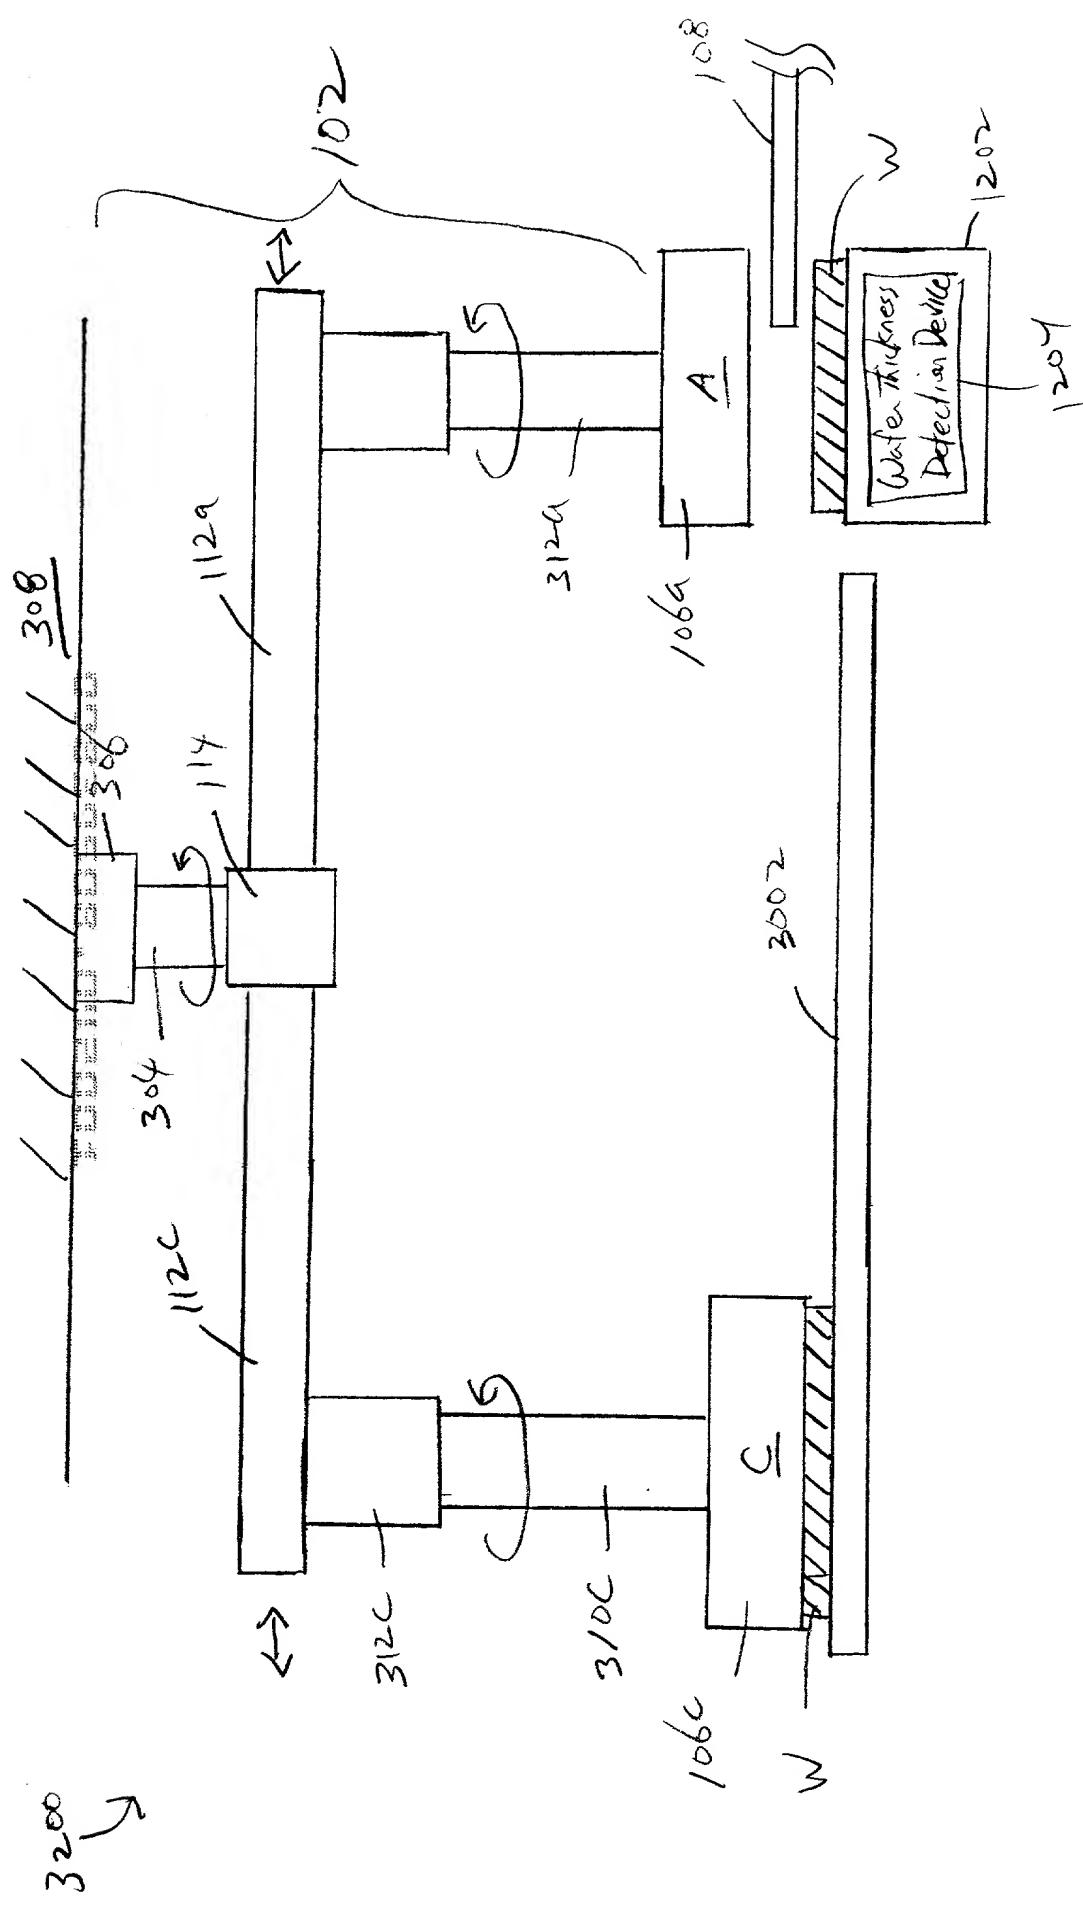



FIG. 3.3

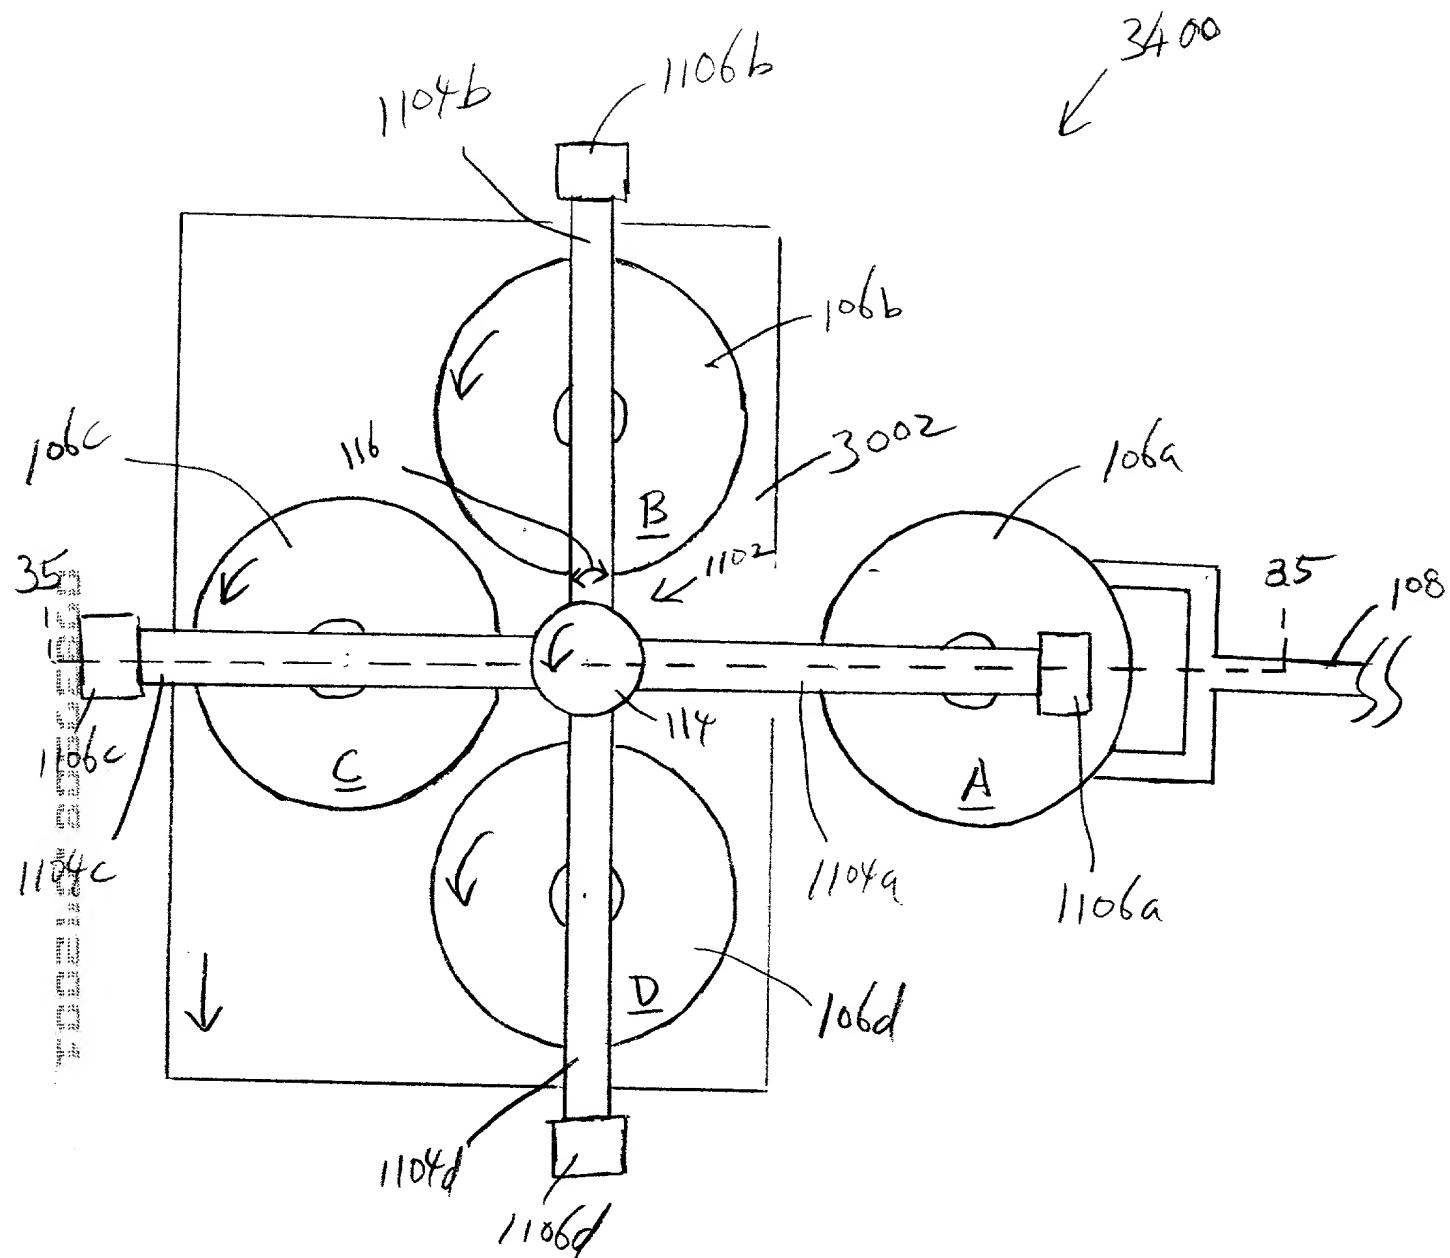

F16 34

ORL-003

FIG. 35

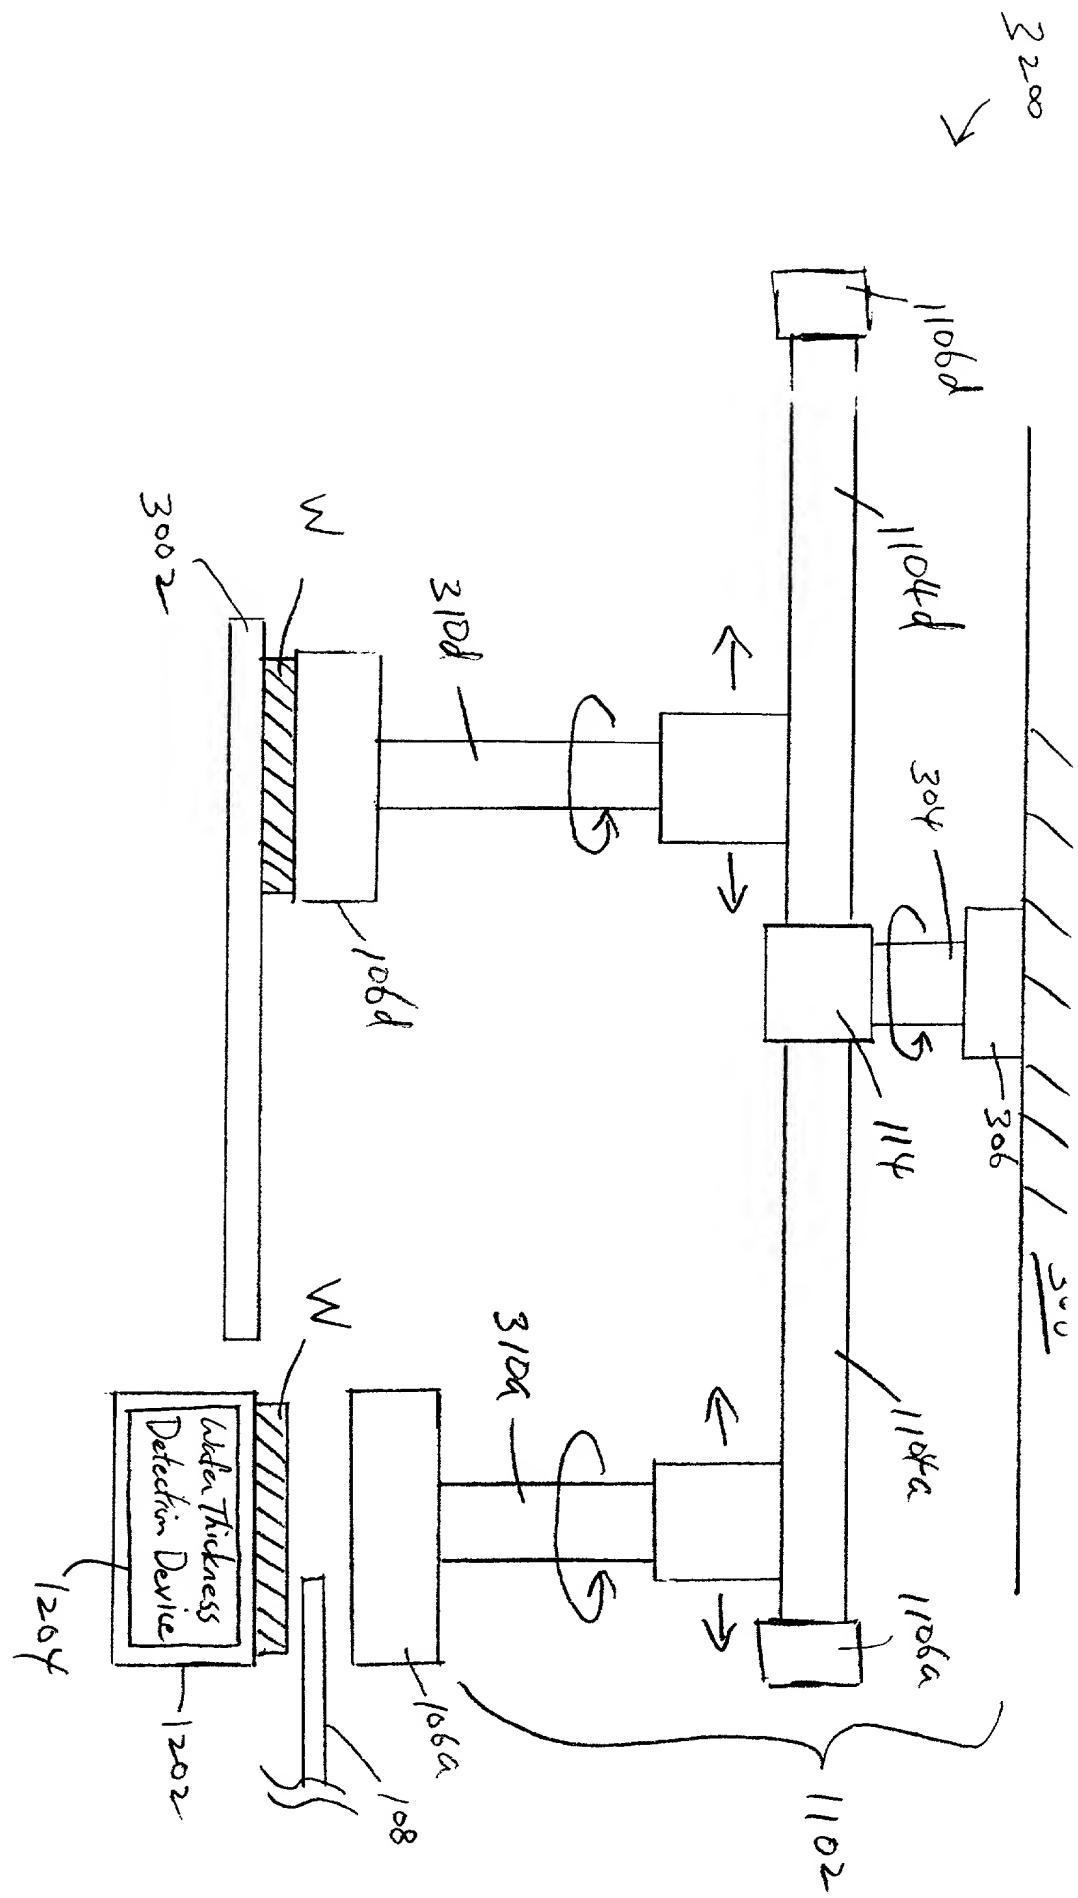

ORL-003

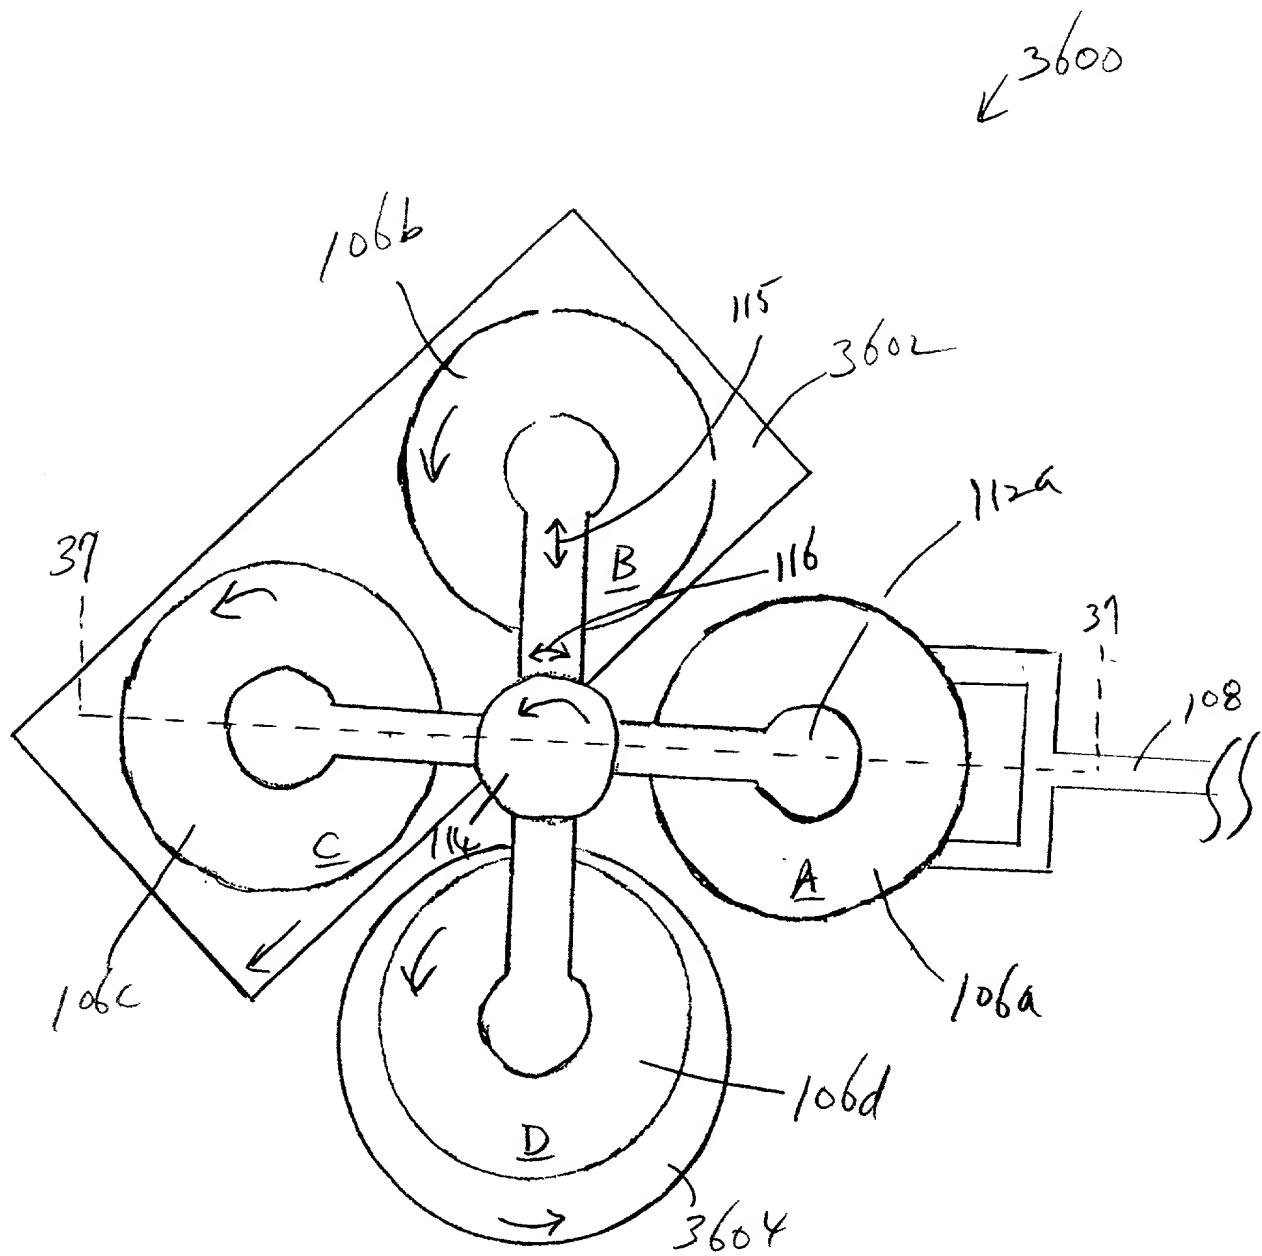


FIG. 36

ORL-003

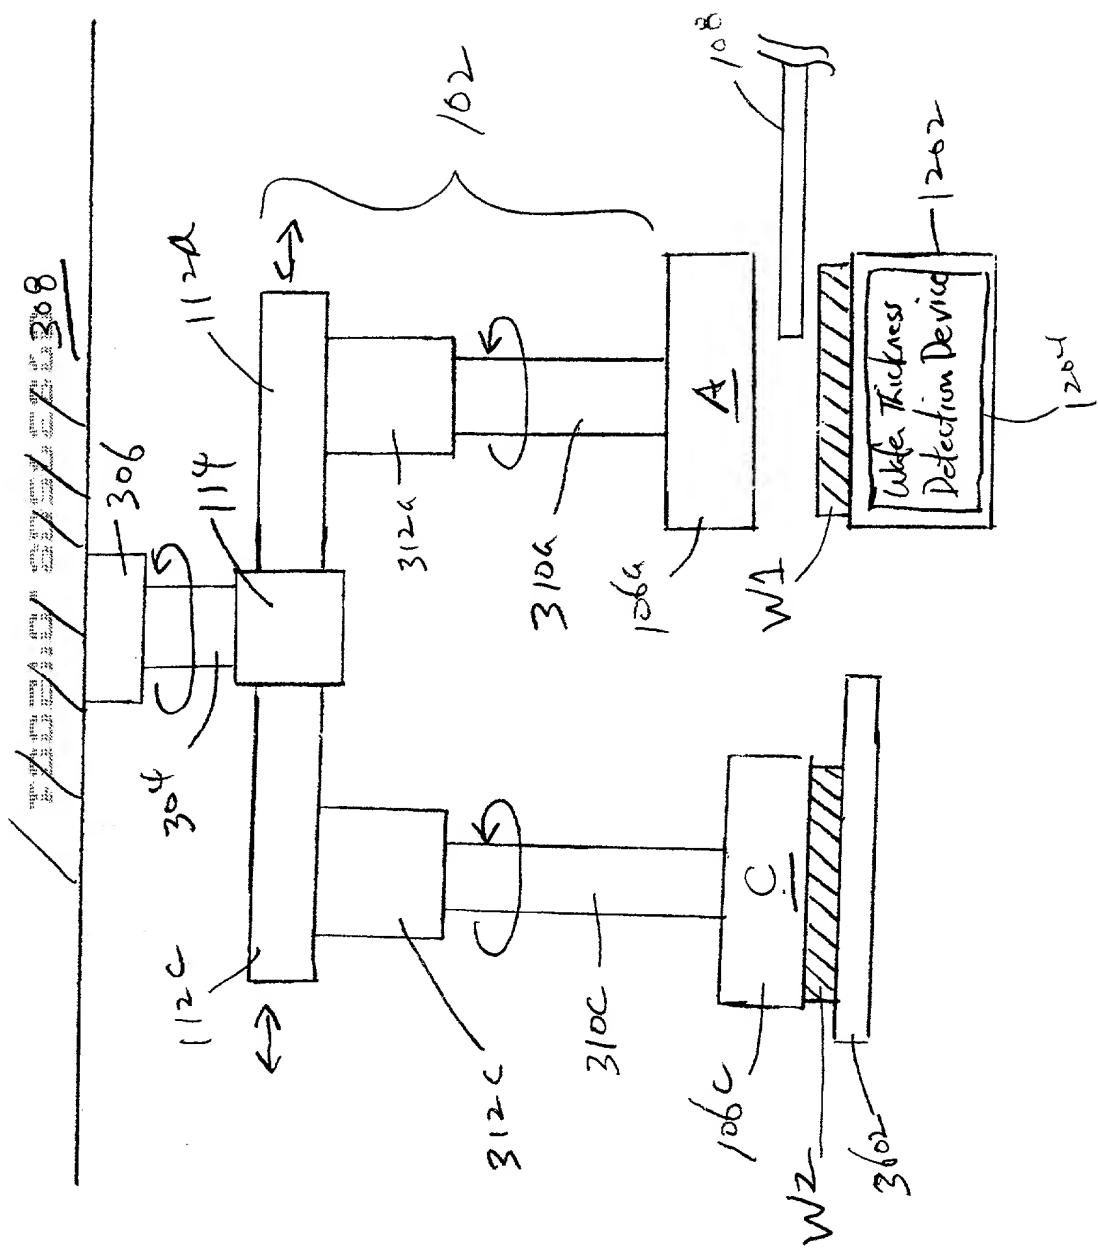


FIG. 31

ORL-003

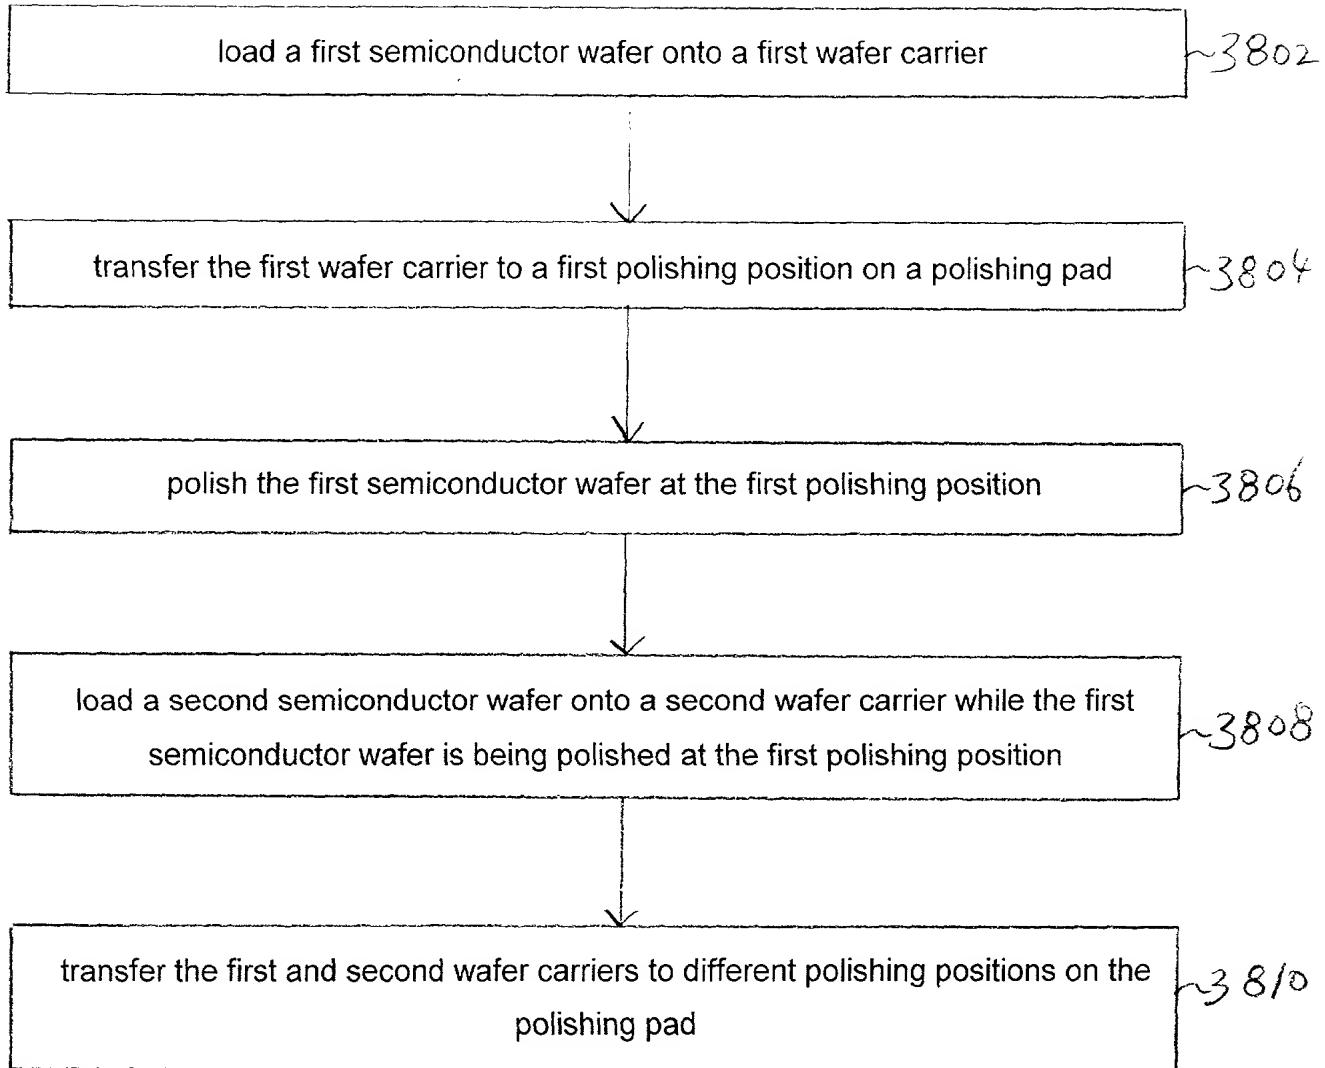


FIG. 38